

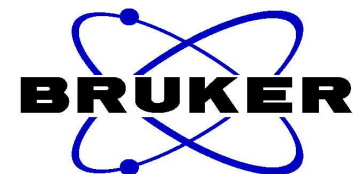


Semax in DMSO-d6  
 AV 400  
 1D Proton Spectrum  
 64 scans  
 April 24, 2015.

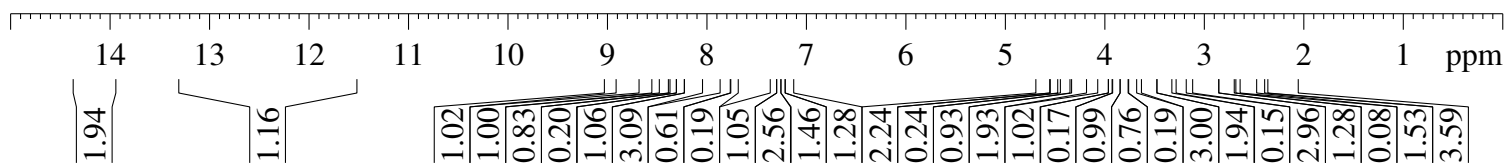


NAME Syn042415  
 EXPNO 21  
 PROCNO 1  
 Date\_ 20150424  
 Time 8.54  
 INSTRUM av400  
 PROBHD 5 mm PABBO BB-  
 PULPROG zg30  
 TD 32768  
 SOLVENT DMSO  
 NS 64  
 DS 0  
 SWH 8278.146 Hz  
 FIDRES 0.252629 Hz  
 AQ 1.9792372 sec  
 RG 1024  
 DW 60.400 usec  
 DE 6.00 usec  
 TE 295.3 K  
 D1 2.50000000 sec  
 TD0 1

===== CHANNEL f1 =====  
 NUC1 1H  
 P1 9.80 usec  
 PL1 0.00 dB  
 PL1W 9.04279137 W  
 SFO1 400.1324710 MHz  
 SI 16384  
 SF 400.1300066 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00

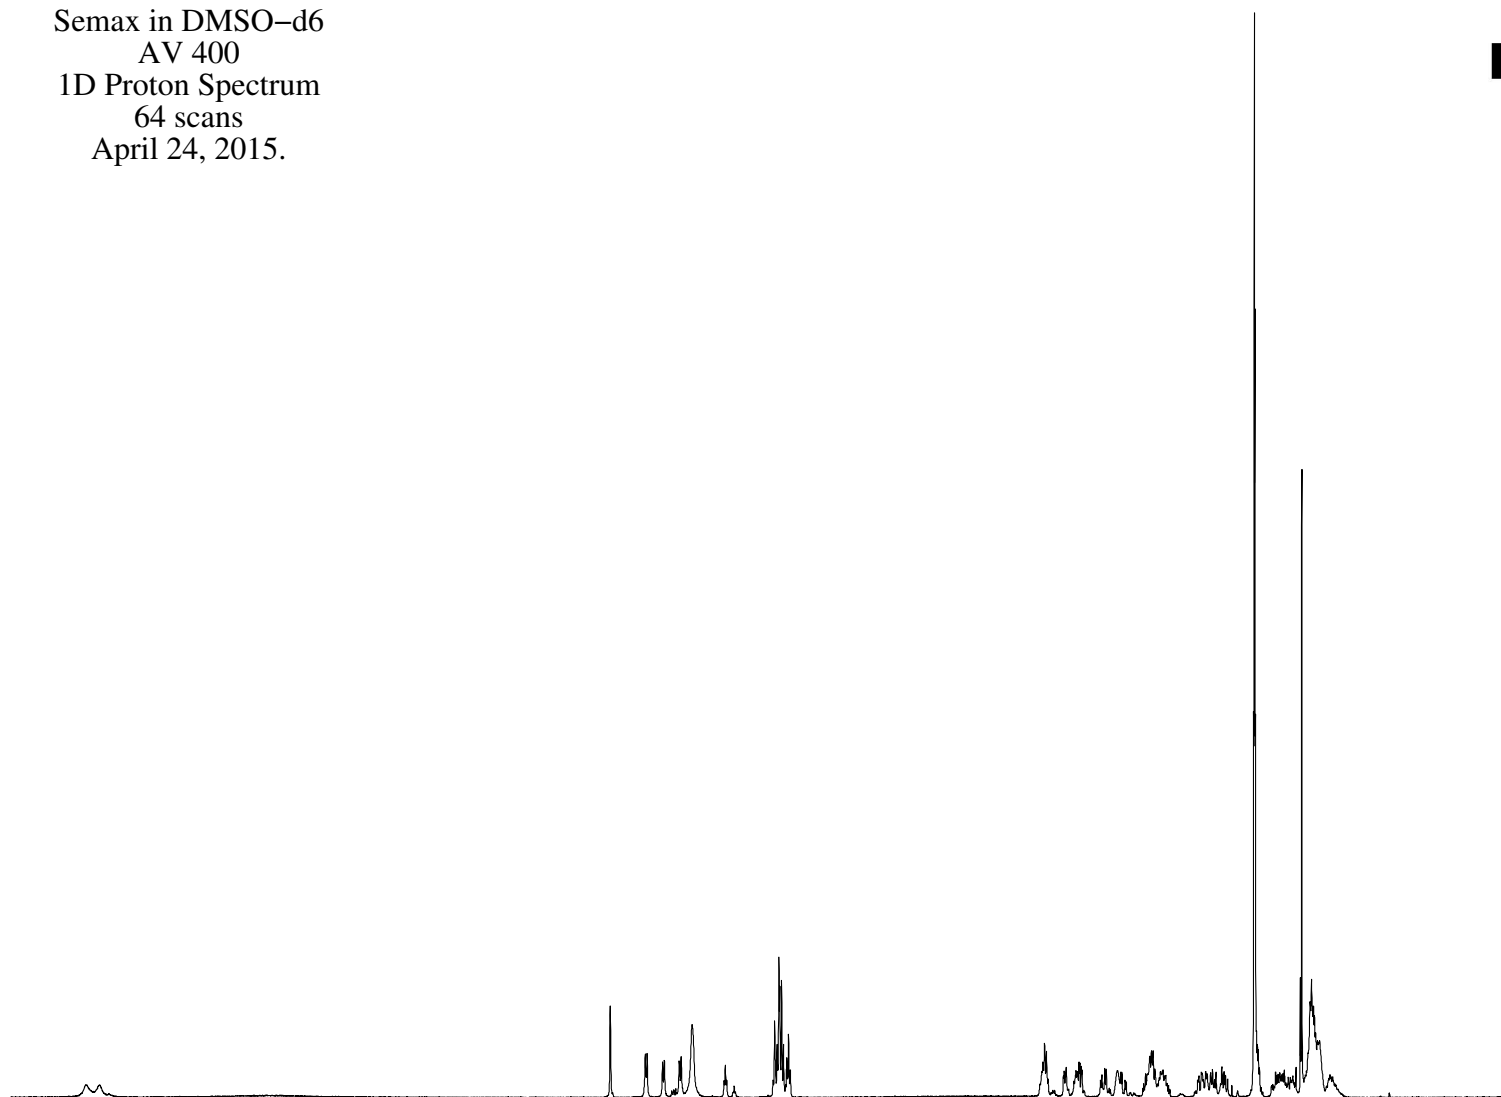

Semax in DMSO-d6  
AV 400  
1D Proton Spectrum  
64 scans  
April 24, 2015.

14.235  
14.098

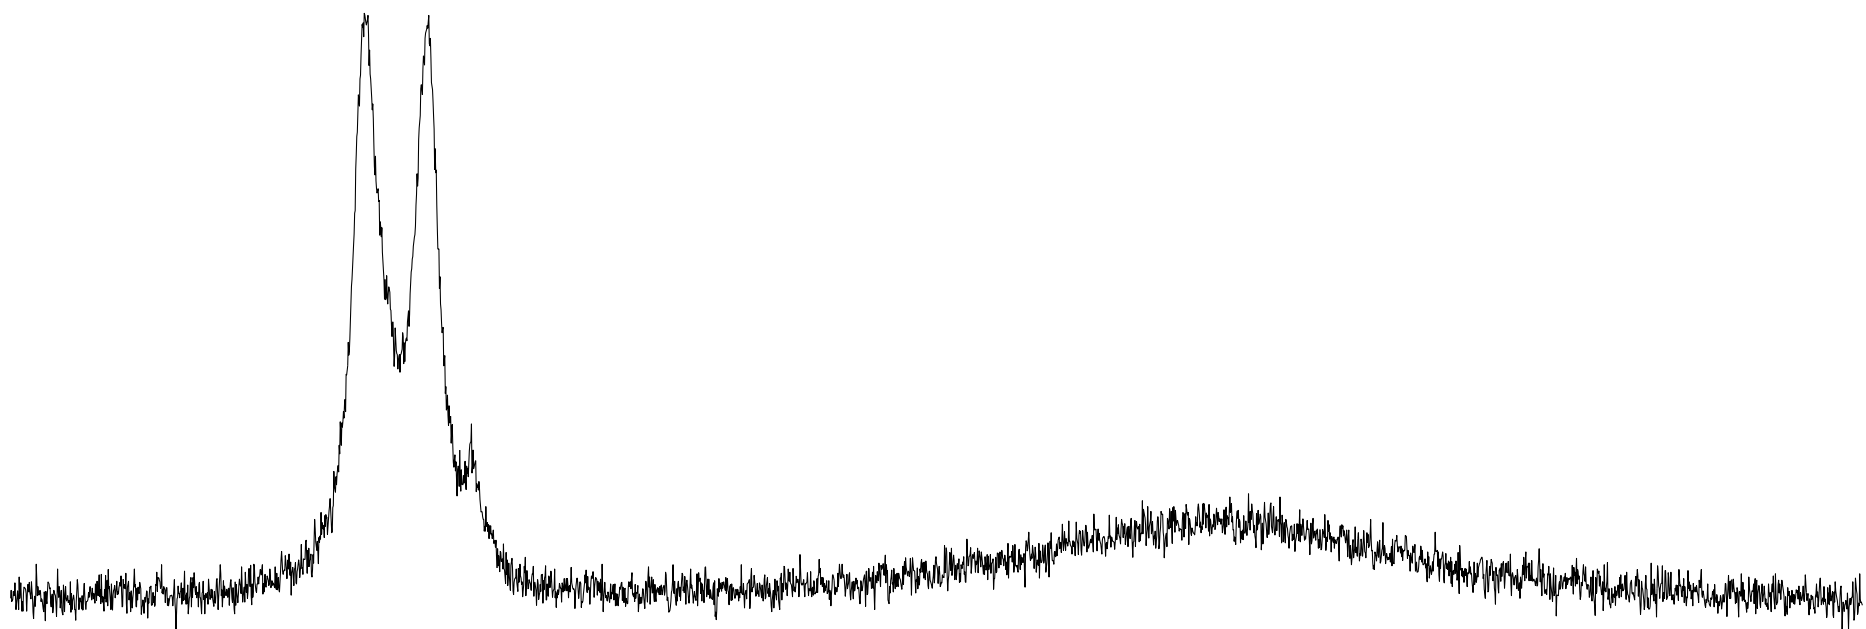

14.5

14.0

13.5

13.0

12.5

12.0


11.5

ppm

1.94



1.16

Semax in DMSO-d6  
AV 400  
1D Proton Spectrum  
64 scans  
April 24, 2015.

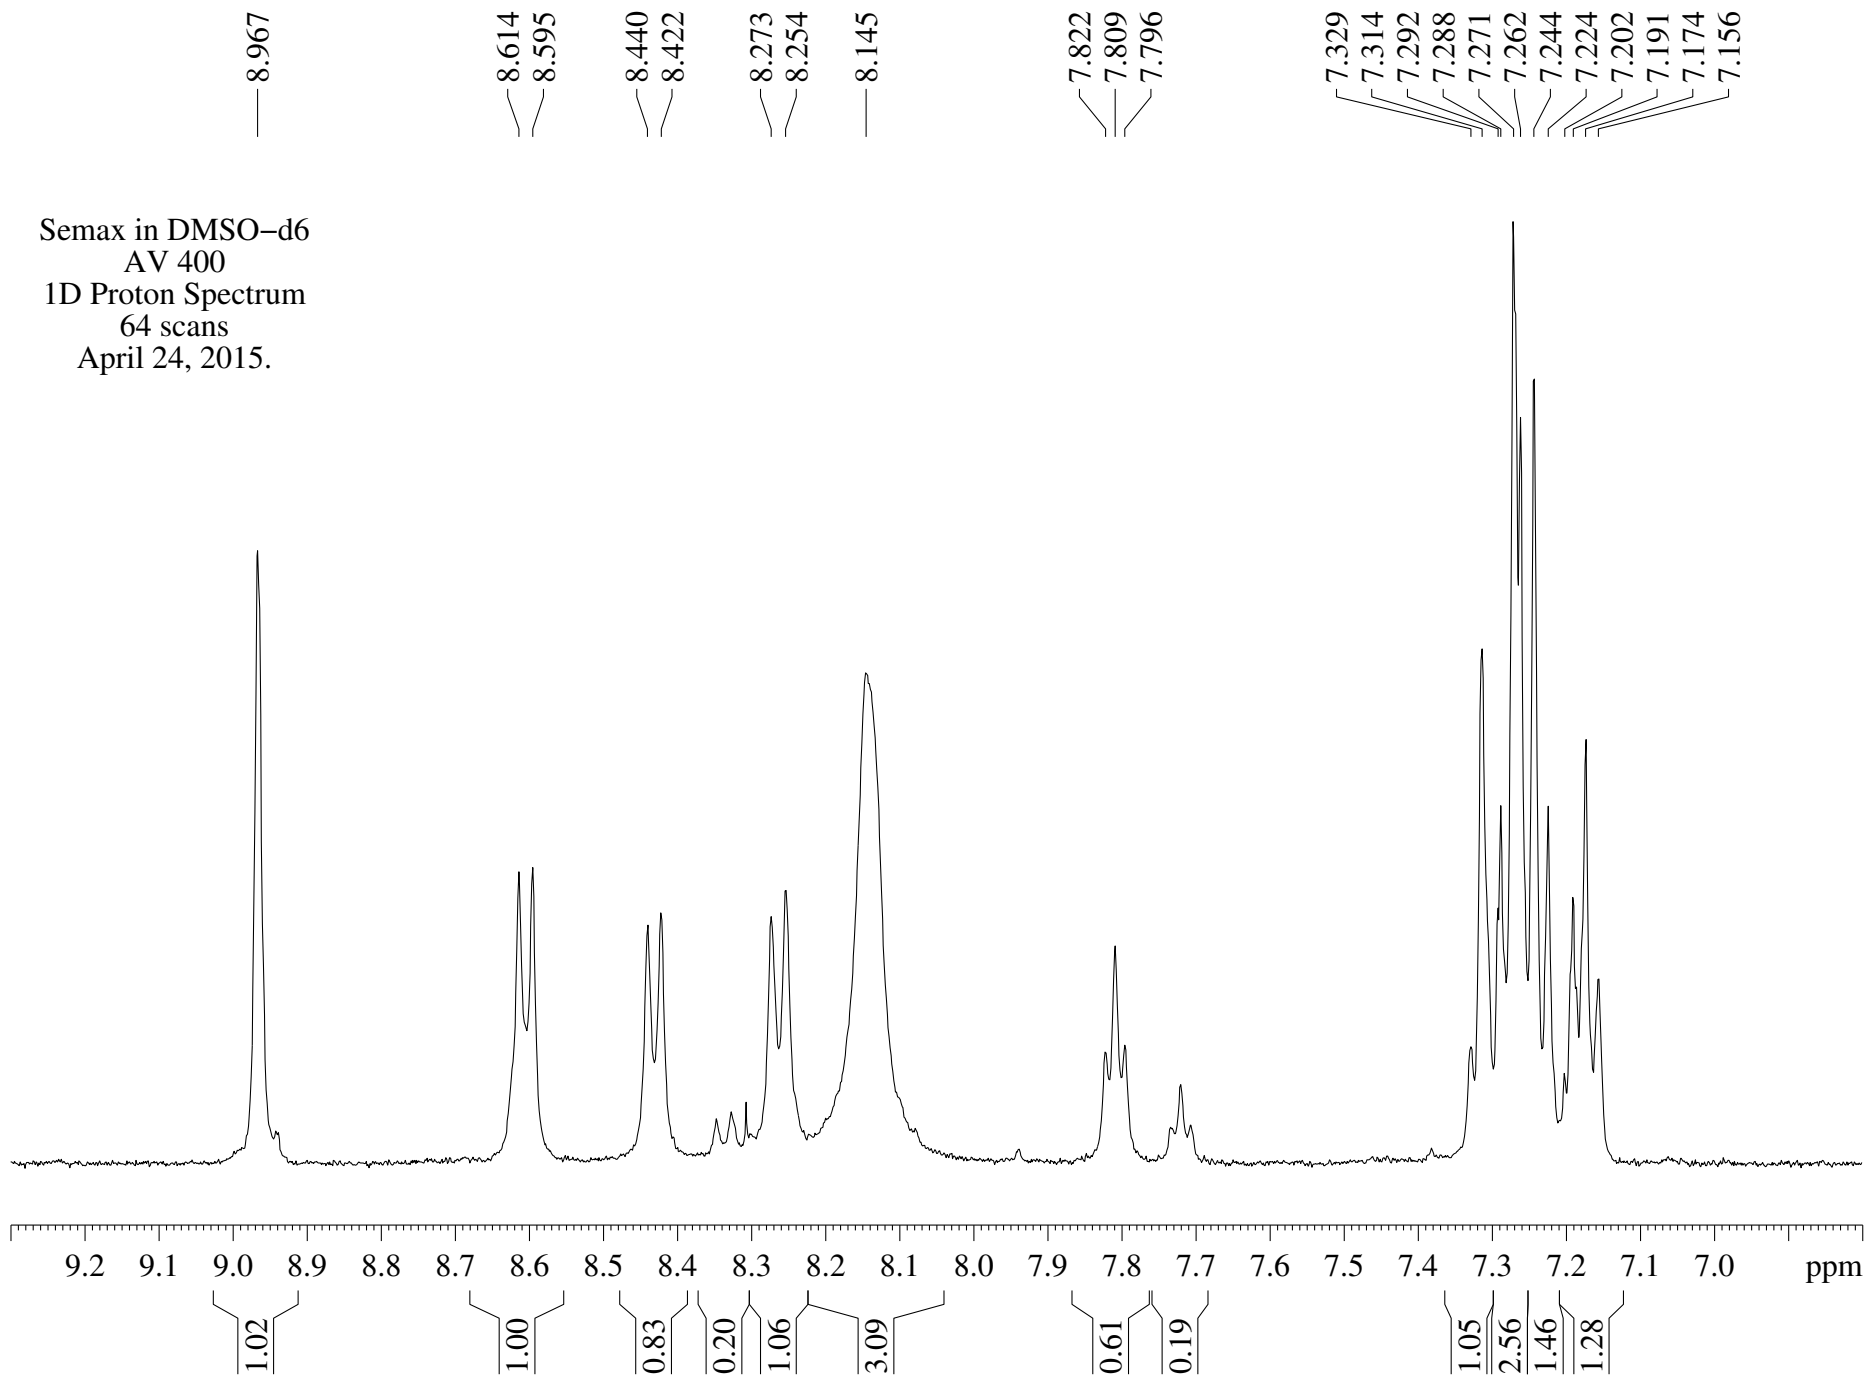

4.625  
4.617  
4.600  
4.581  
4.564  
4.410  
4.403  
4.391  
4.383  
4.284  
4.272  
4.254  
4.246  
4.232  
4.224  
4.023  
3.994  
3.980  
3.868  
3.835  
3.822  
3.586  
3.577  
3.569  
3.539  
3.526  
3.518  
3.509  
3.491  
3.446  
3.433  
3.426  
3.417  
3.408  
3.393  
3.386  
3.382  
3.048  
3.025  
3.014  
3.005  
2.981  
2.966  
2.931  
2.913  
2.892  
2.877  
2.817  
2.796  
2.783  
2.761

Semax in DMSO-d6  
AV 400  
1D Proton Spectrum  
64 scans  
April 24, 2015.

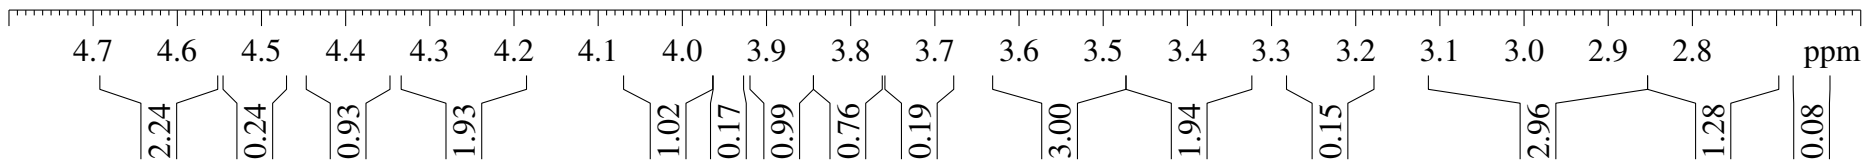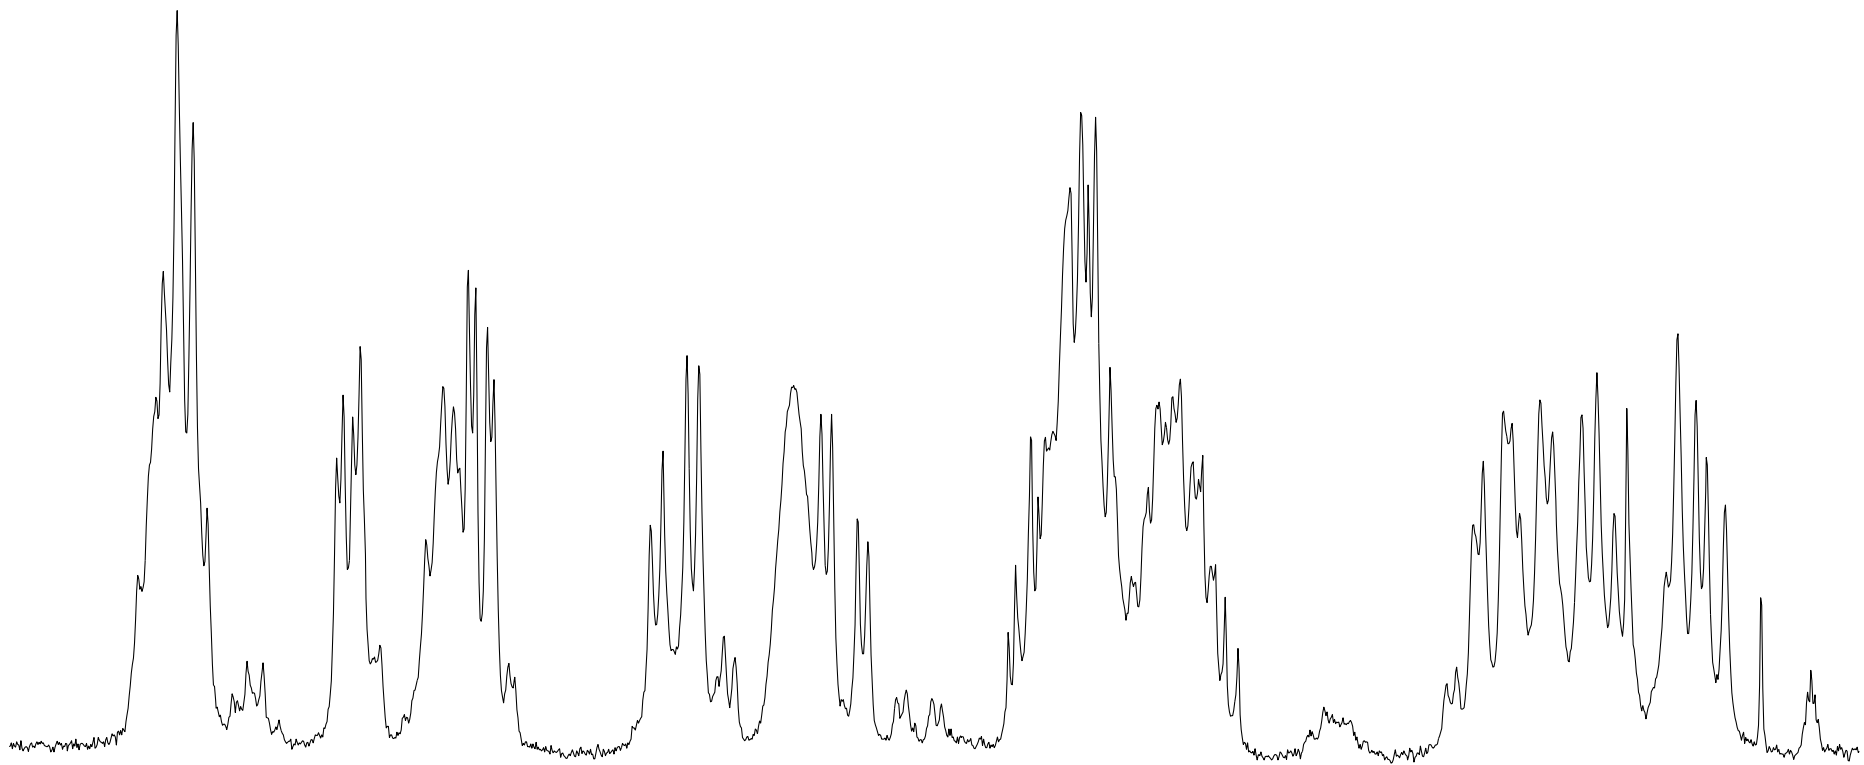

Semax in DMSO-d6  
AV 400  
1D Proton Spectrum  
64 scans  
April 24, 2015.

