


LDsB Maleate in DMSO-d6
NEO 400
1D Proton Spectrum
November 27, 2024.

Current Data Parameters
NAME Syntharise112724
EXPNO 400
PROCNO 1


F2 - Acquisition Parameters
Date_ 20241127
Time 13.43 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 (
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 297.2 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters
SI 65536
SF 400.340068 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

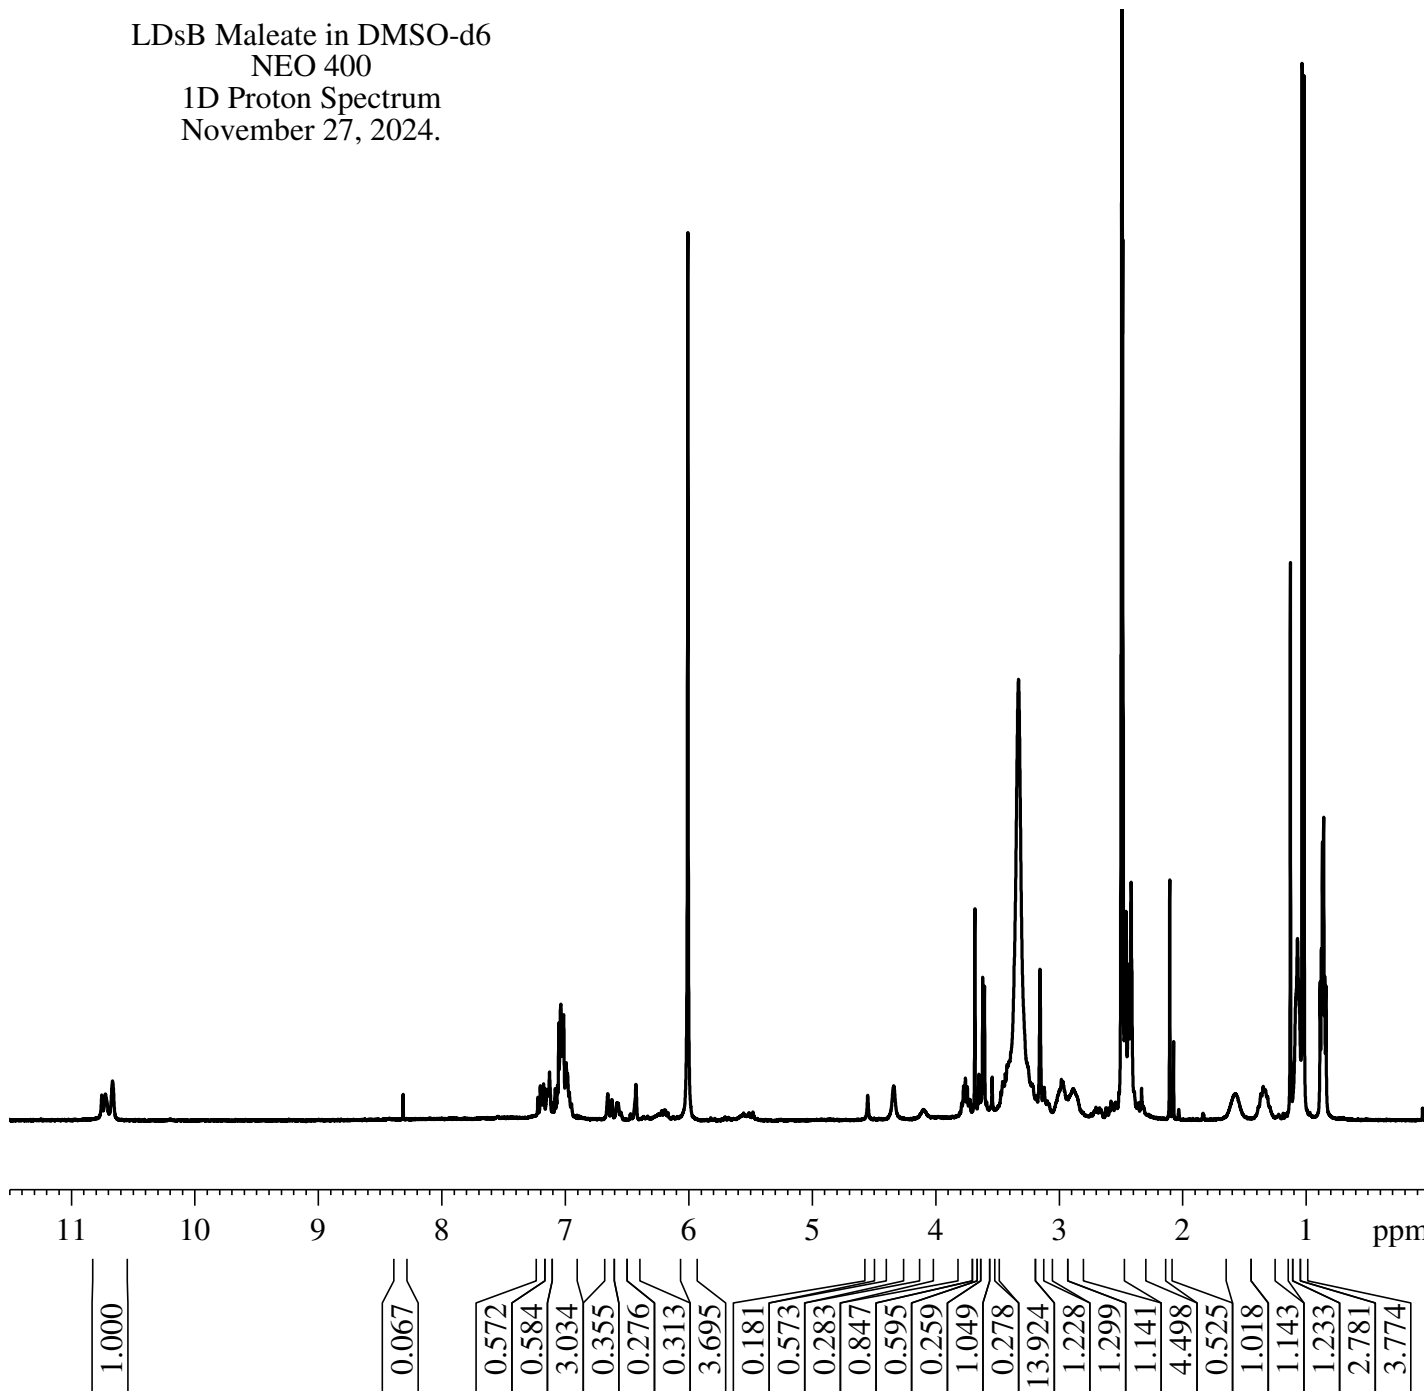


LDsB Maleate in DMSO-d6
NEO 400
1D Proton Spectrum
November 27, 2024.


— 10.754
— 10.725
— 10.667

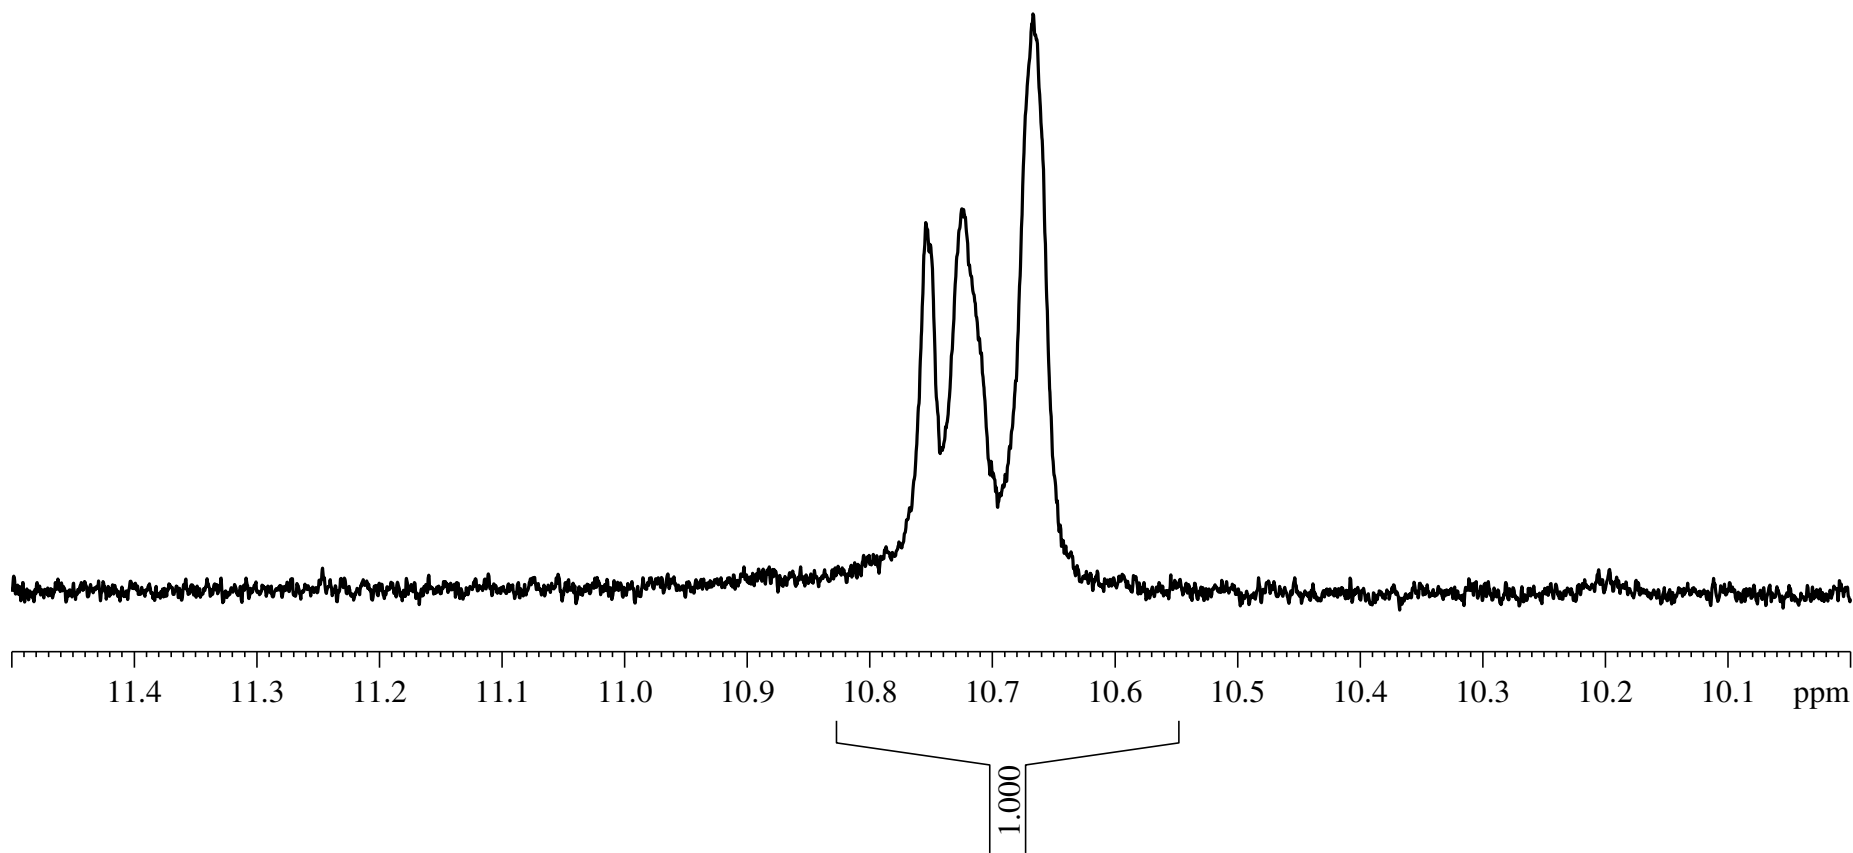

LDsB Maleate in DMSO-d6
NEO 400
1D Proton Spectrum
November 27, 2024.

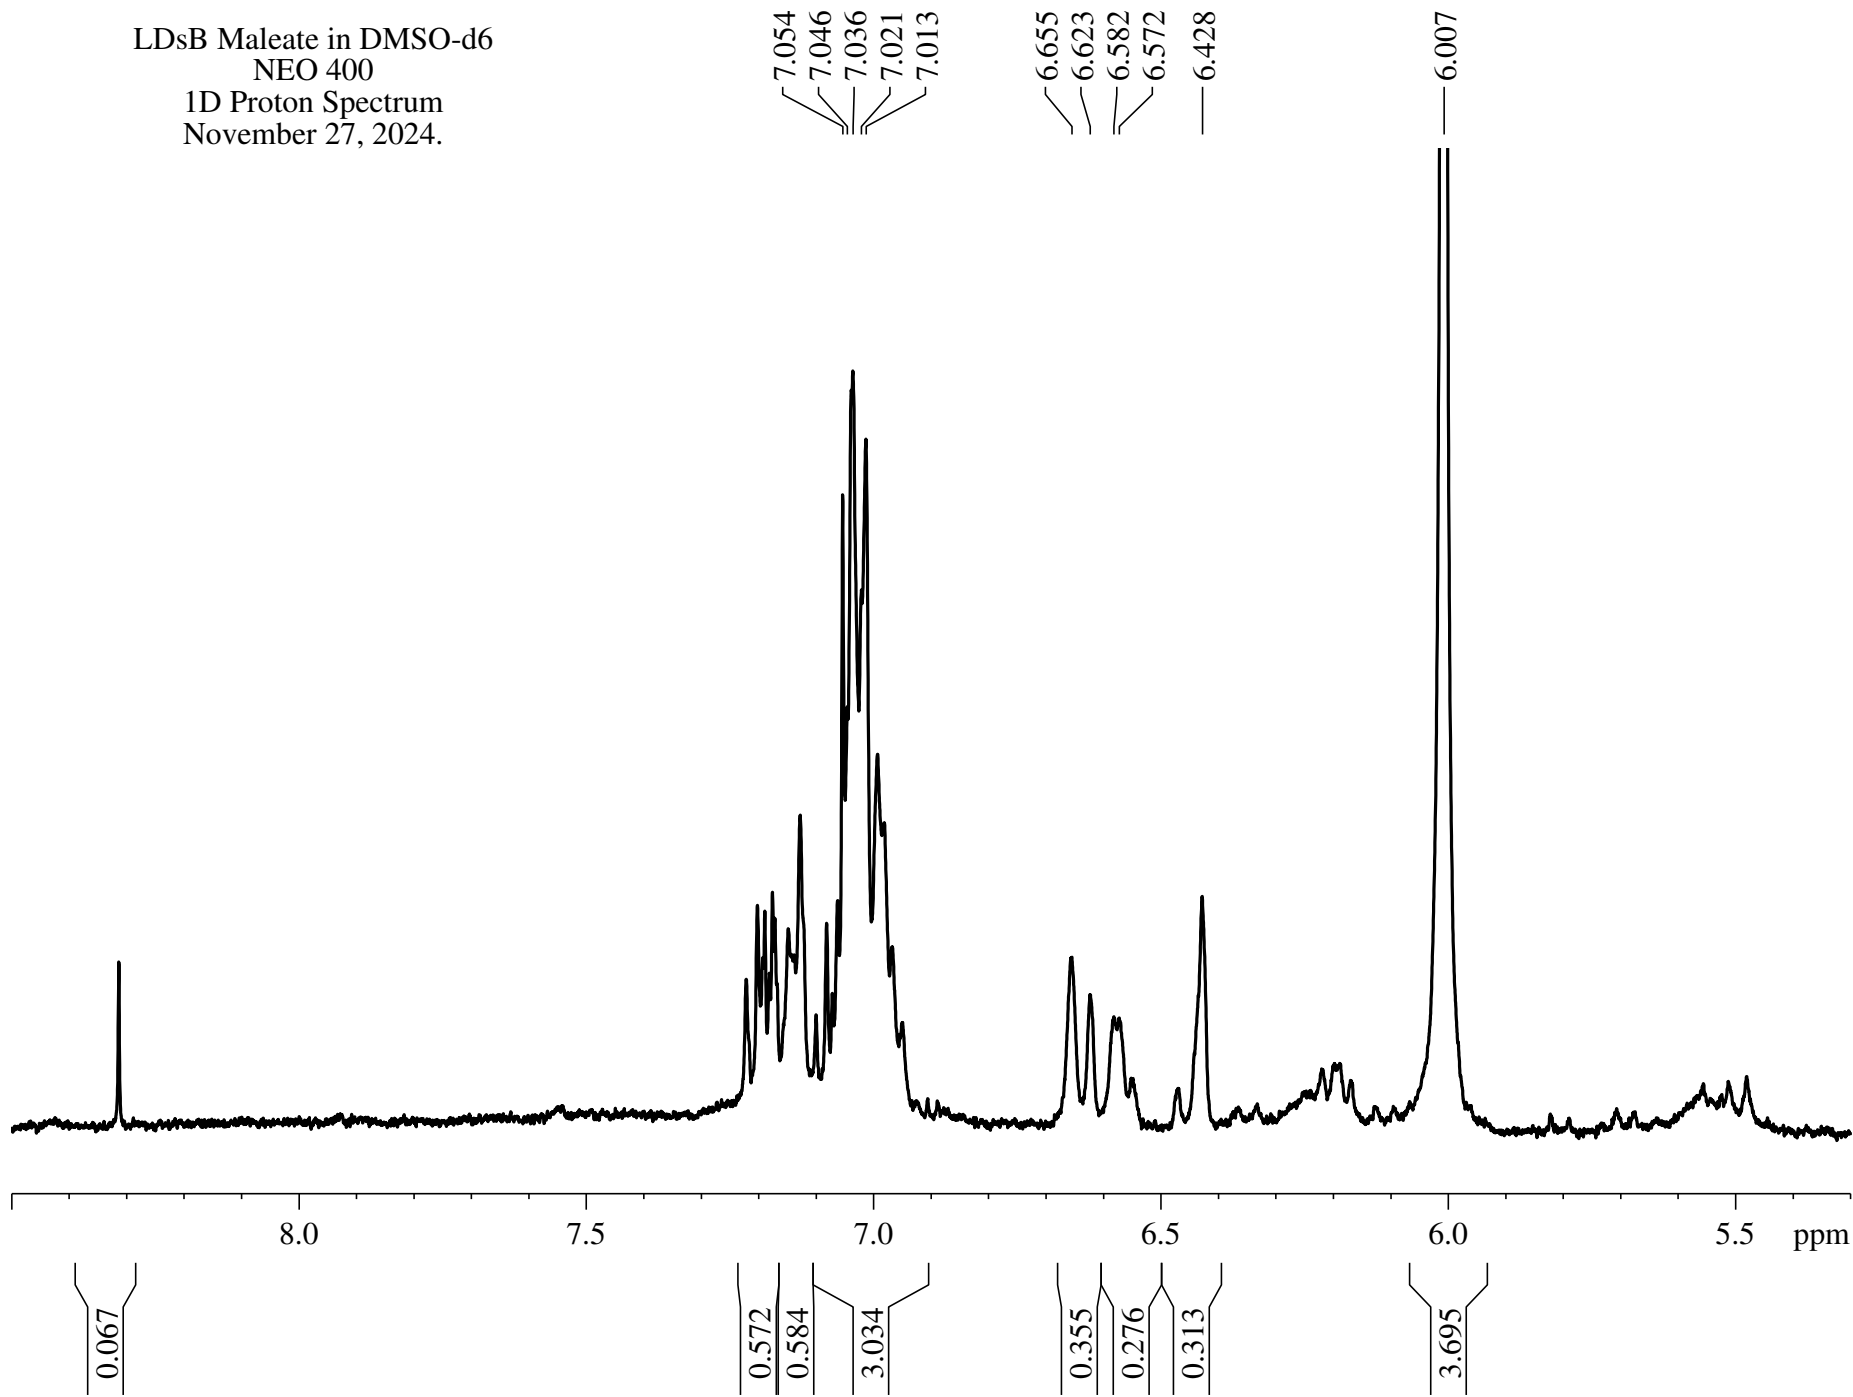


LDsB Maleate in DMSO-d6
NEO 400
1D Proton Spectrum
November 27, 2024.

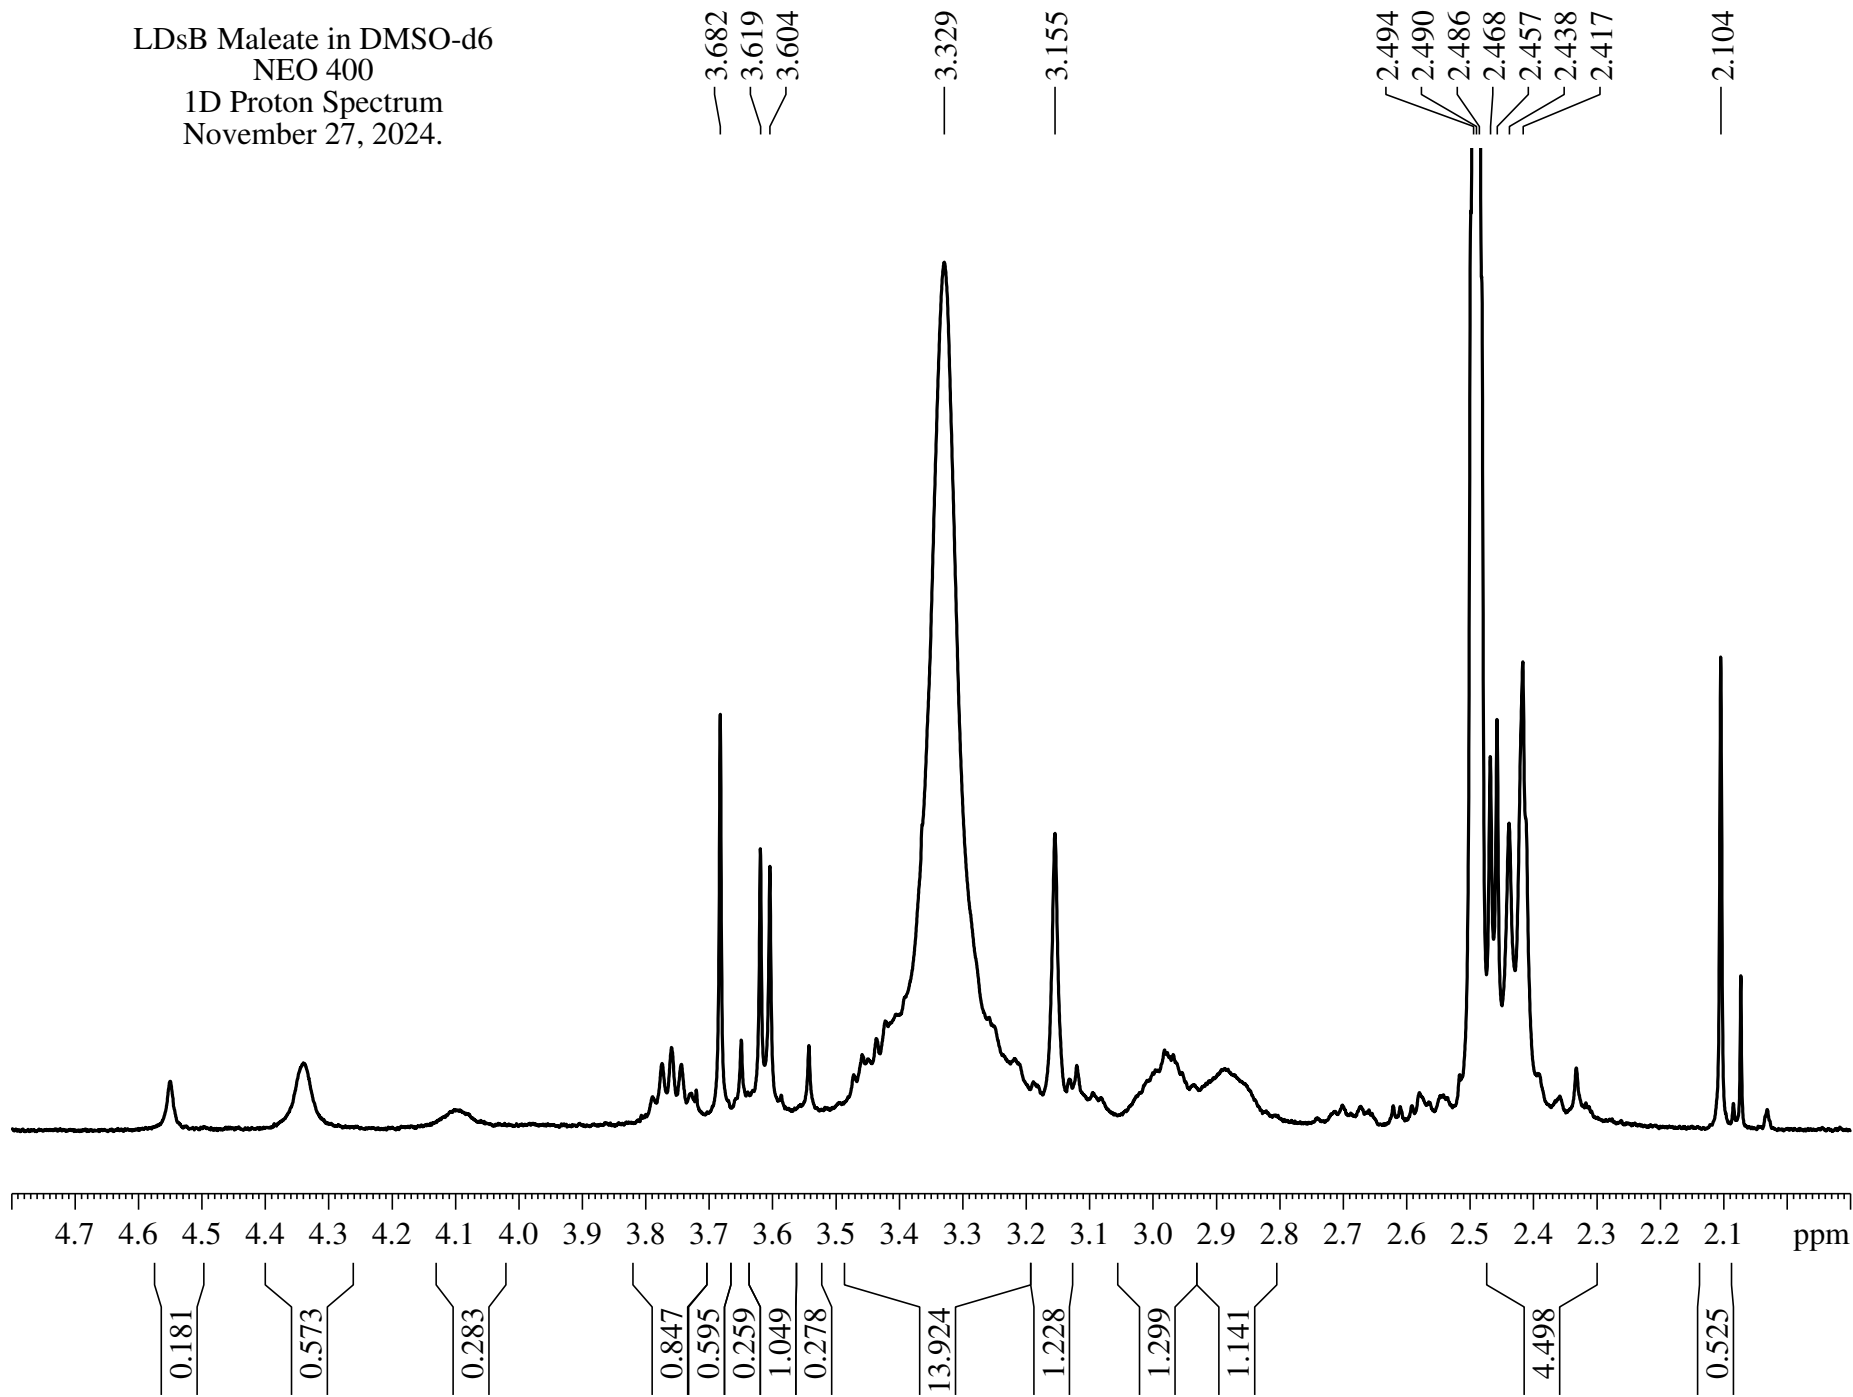

LDsB Maleate in DMSO-d6
NEO 400
1D Proton Spectrum
November 27, 2024.

— 1.127
— 1.069
— 1.032
— 1.016
— 0.886
— 0.876
— 0.867
— 0.857
— 0.849
— 0.839

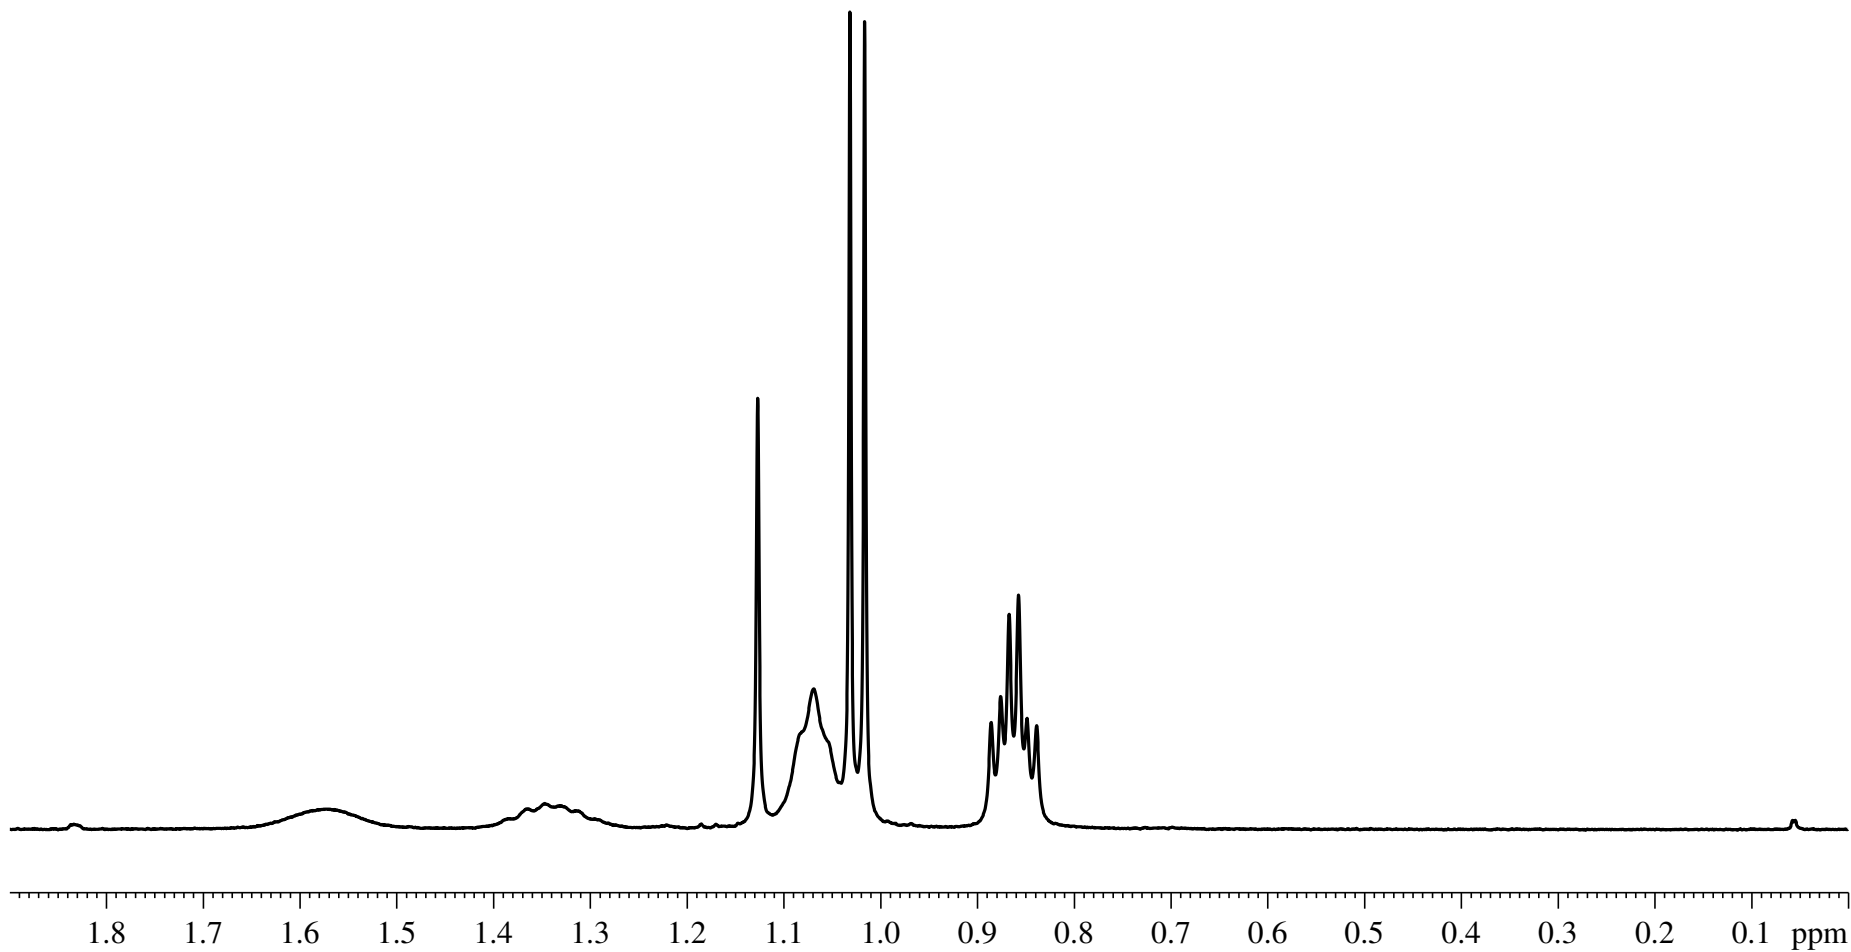

1.018
1.143
1.233
2.781
3.774
3.493