


METHYLENEDIOXYISOPROPAMPHPROAMINEHYDROCHLOR

Sample 2 in DMSO-d6
NEO 400
1D Proton Spectrum
January 8, 2025.

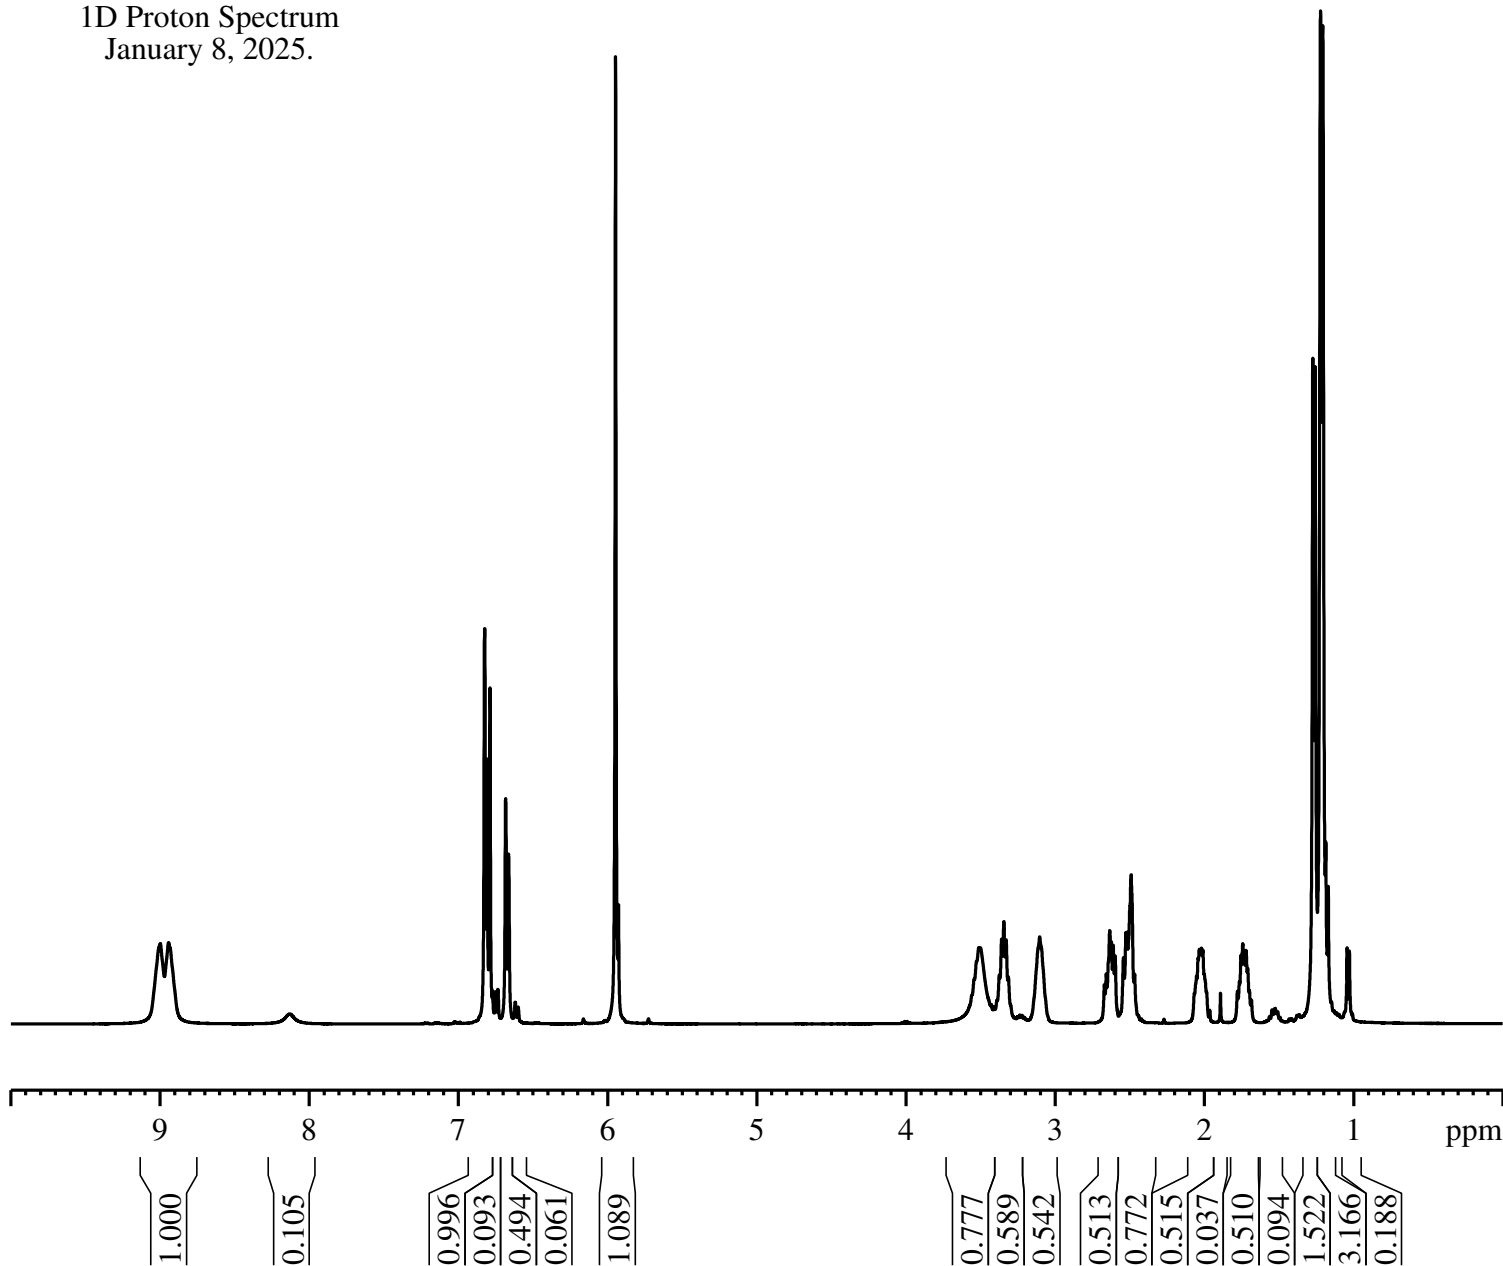

Current Data Parameters

NAME Syntharise010825
EXPNO 440
PROCNO 1


F2 - Acquisition Parameters

Date_ 20250108
Time 14.28 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 (PI HR-400-S)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 7
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 36.059
DW 61.000 usec
DE 13.54 usec
TE 295.5 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters

SI 65536
SF 400.3400068 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

Sample 2 in DMSO-d6
NEO 400
1D Proton Spectrum
January 8, 2025.

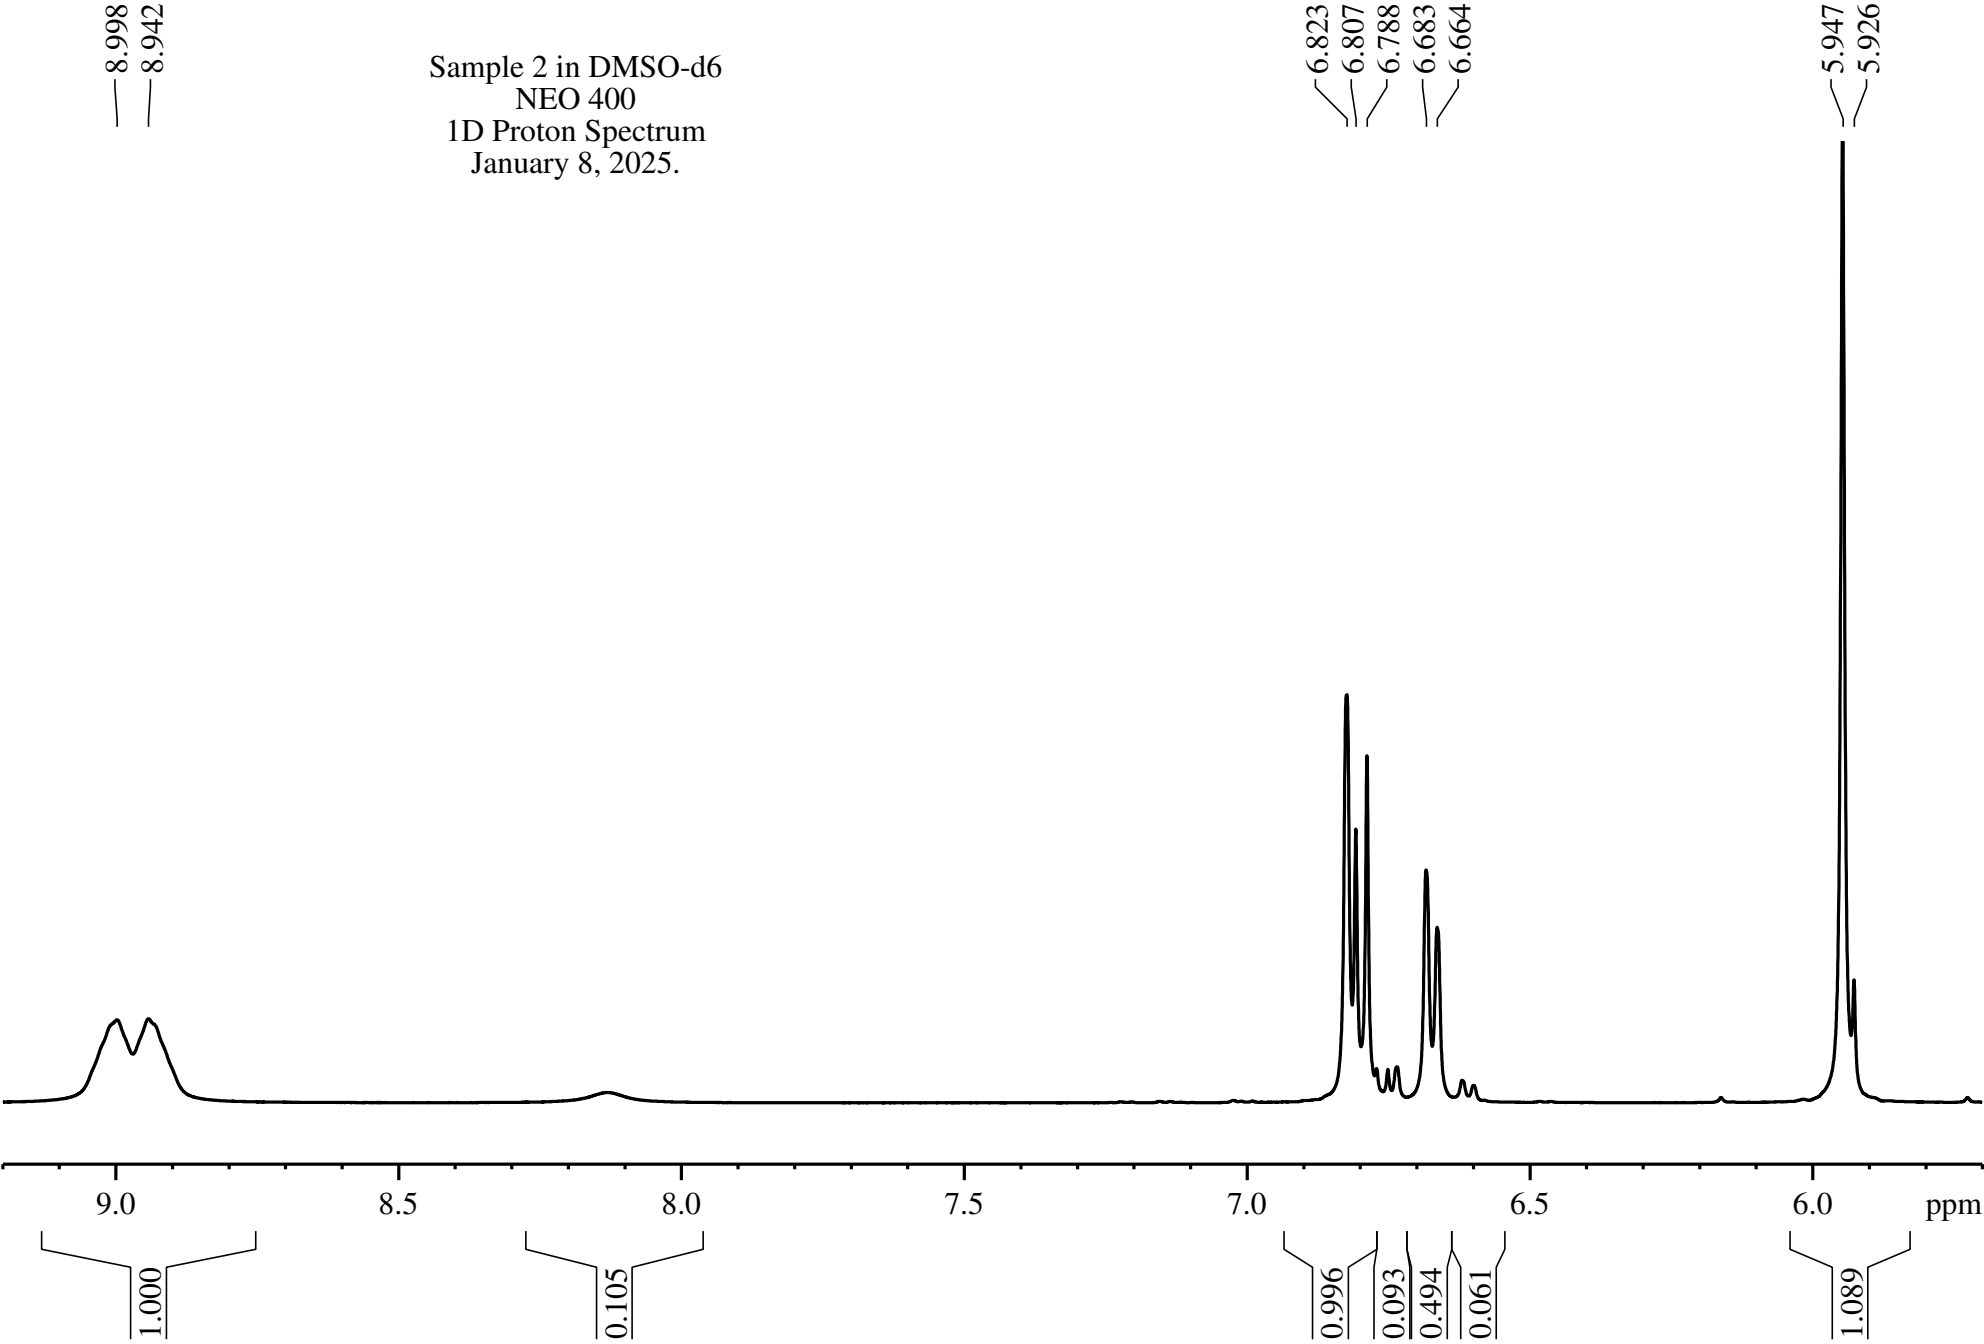

3.512
3.503
3.359
3.344
3.329

— 3.104


2.634
2.623
2.610
2.598
2.543
2.526
2.518
2.490

2.042
2.034
2.026
2.018
2.010

1.754
1.742
1.732
1.721

1.273
1.257
1.221
1.207
1.186
1.170
1.043
1.028

Sample 2 in DMSO-d6
NEO 400
1D Proton Spectrum
January 8, 2025.

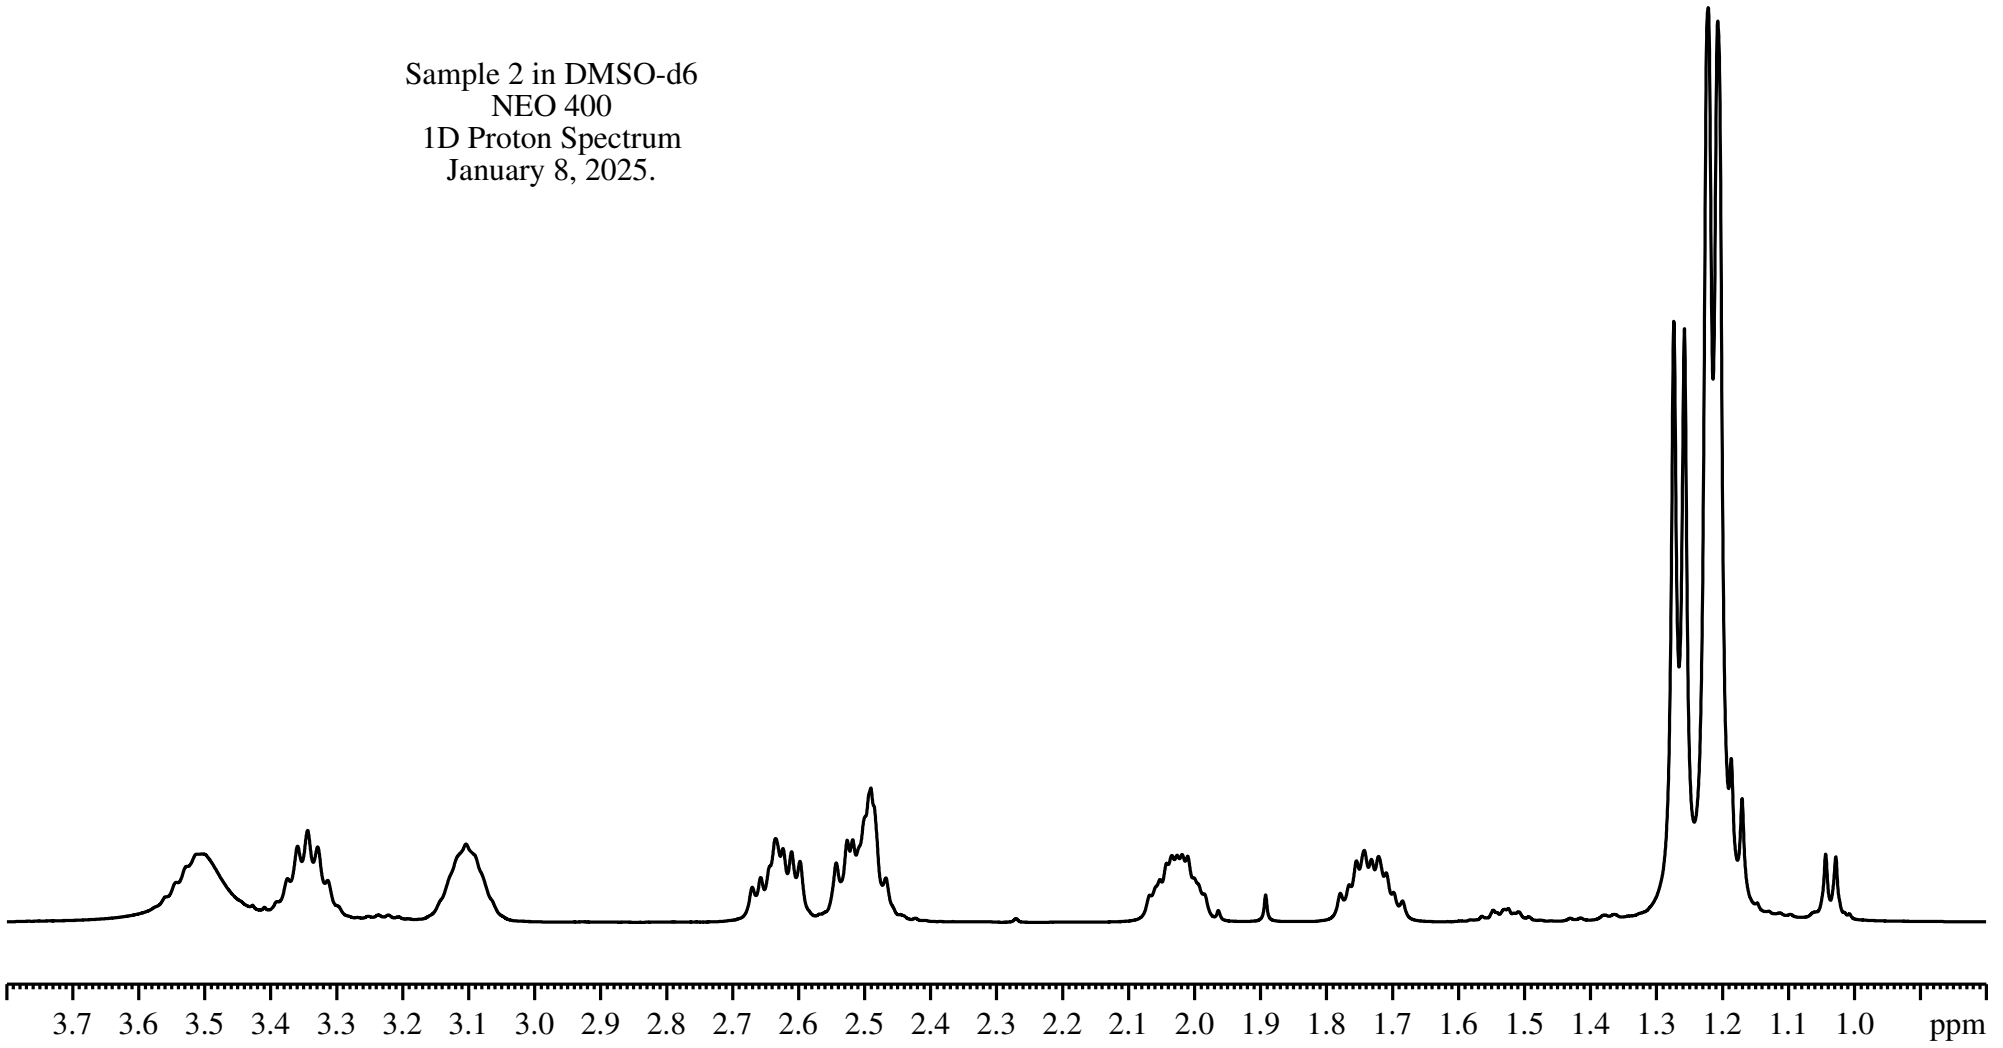

0.777
0.589
0.542
0.513
0.772
0.515
0.037
0.510
0.094
1.522
3.166
0.188