

Confirmed correct !

NPP in DMSO-d6
Isopropamphroamine (HCl)
NEO 400
1D Proton Spectrum
January 8, 2025.

Current Data Parameters


NAME Syntharise010825
EXPNO 400
PROCNO 1

F2 - Acquisition Parameters

Date_ 20250108
Time 14.18 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 (PI HR-400-S)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 295.4 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters


SI 65536
SF 400.3400067 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

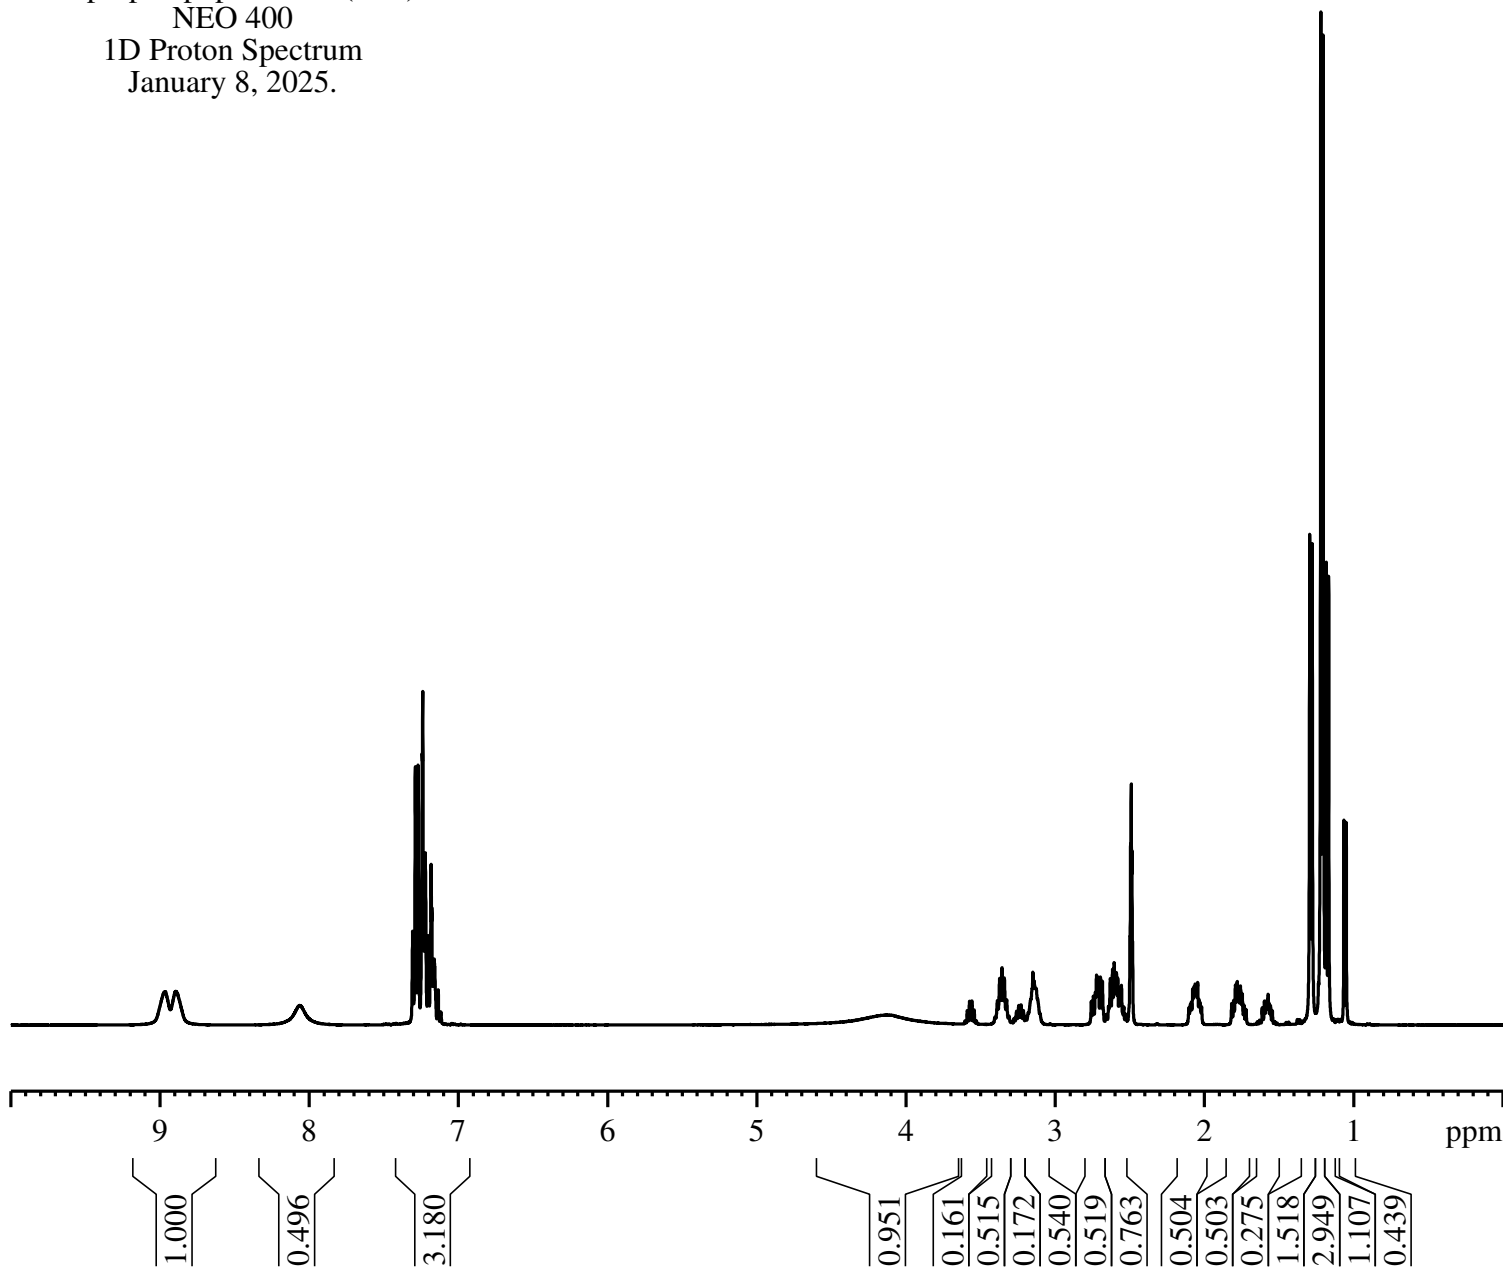

NPP in DMSO-d6
Isopropamphproamine (HCl)
NEO 400
1D Proton Spectrum
January 8, 2025.

— 8.965
— 8.896

7.288
7.270
7.242
7.239
7.222

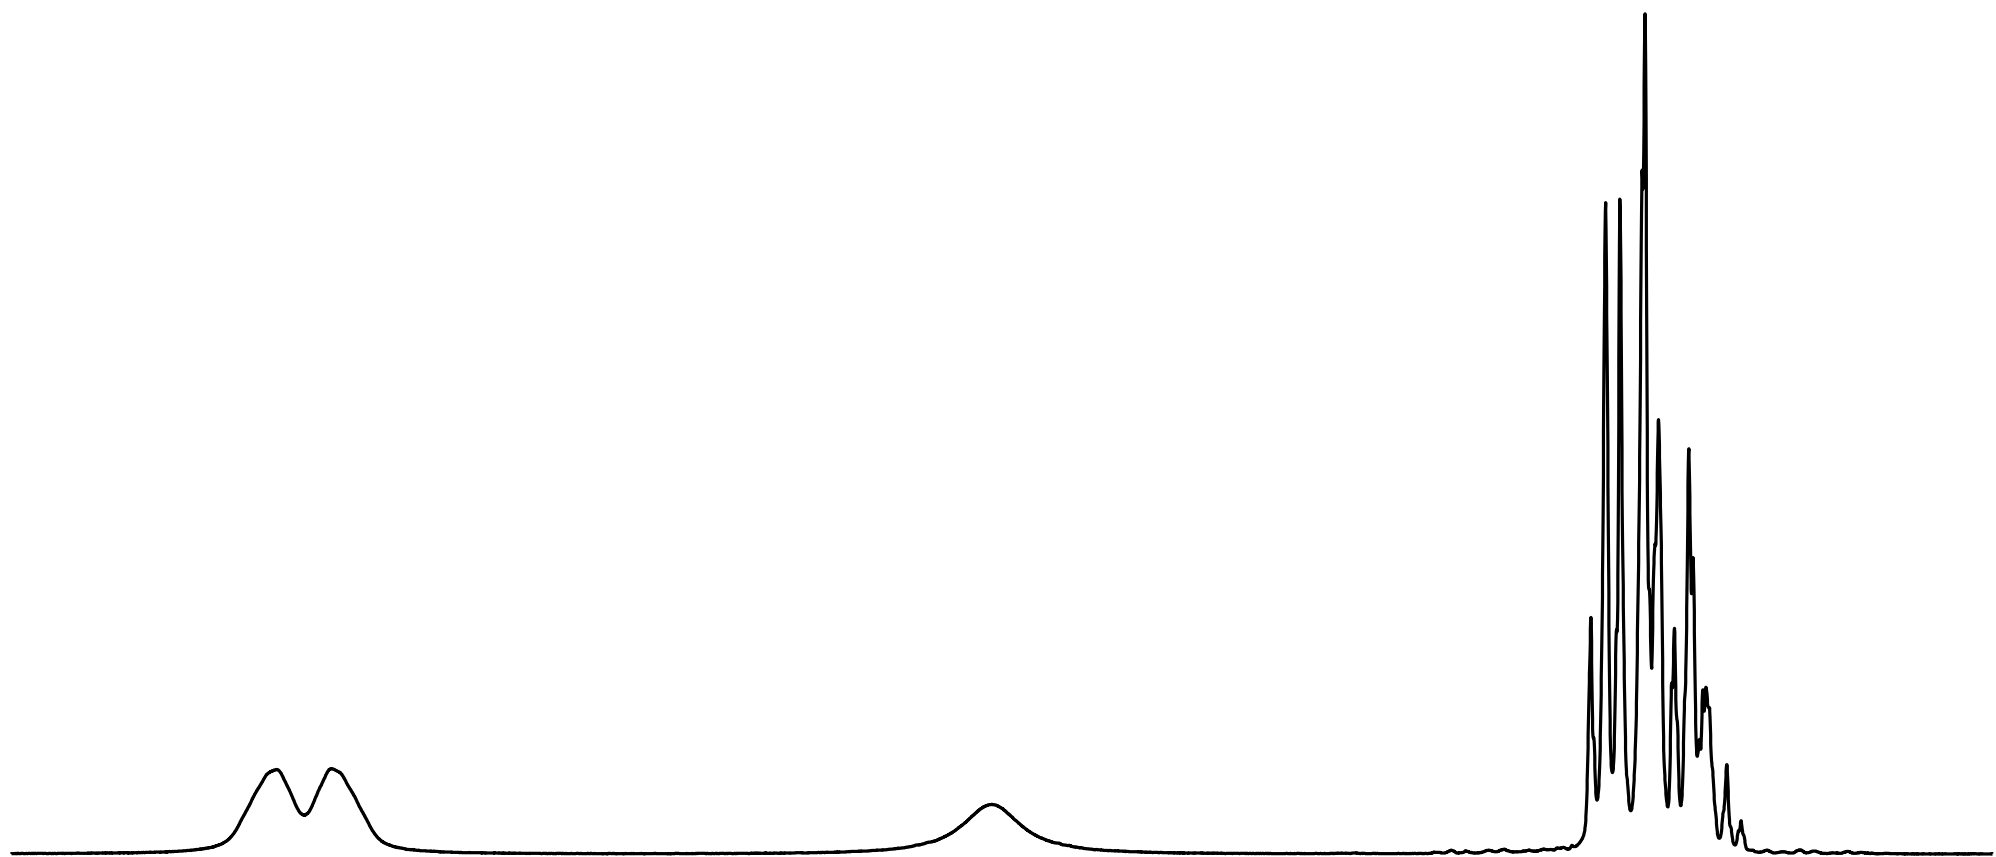

9.2 9.1 9.0 8.9 8.8 8.7 8.6 8.5 8.4 8.3 8.2 8.1 8.0 7.9 7.8 7.7 7.6 7.5 7.4 7.3 7.2 7.1 7.0 ppm

1.000

0.496

3.180

NPP in DMSO-d6
Isopropamphroamine (HCl)
NEO 400
1D Proton Spectrum
January 8, 2025.


4.144
4.120
4.104
4.089

3.574
3.558

3.372
3.356
3.341

3.149
3.141

2.723
2.710
2.697
2.684
2.631
2.615
2.605
2.597
2.589
2.581
2.556
2.499
2.494
2.490

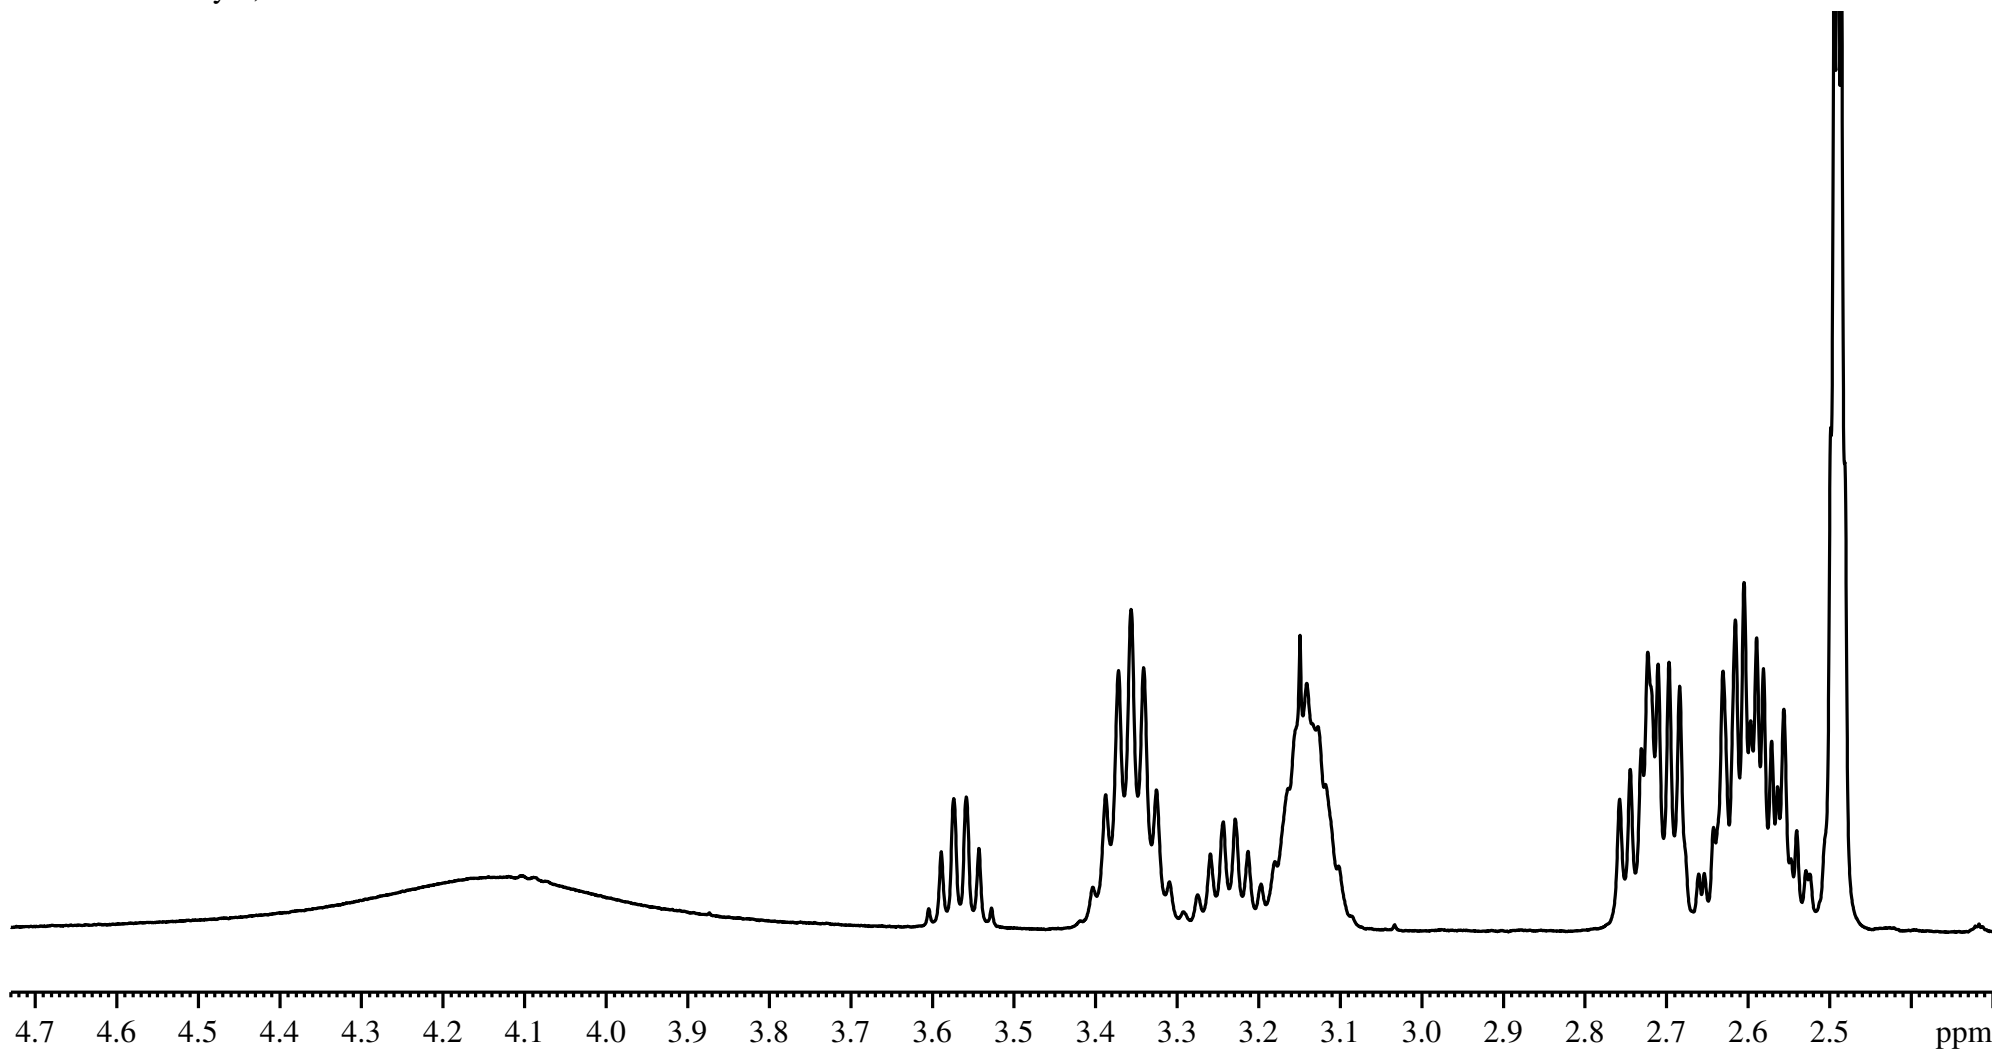

0.951
0.161
0.515
0.172
0.540

0.519
0.763

NPP in DMSO-d6
Isopropamphroamine (HCl)
NEO 400
1D Proton Spectrum
January 8, 2025.

