


Desoxy-D2PM HCl in DMSO-d6
NEO 400
1D Proton Spectrum
April 5, 2024.

Current Data Parameters
NAME Syntharise030524
EXPNO 430
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240405
Time 13.34 h
INSTRUM Avance Neo 400
PROBHD Z104450_0313 (
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 299.6 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W



F2 - Processing parameters
SI 65536
SF 400.3400053 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

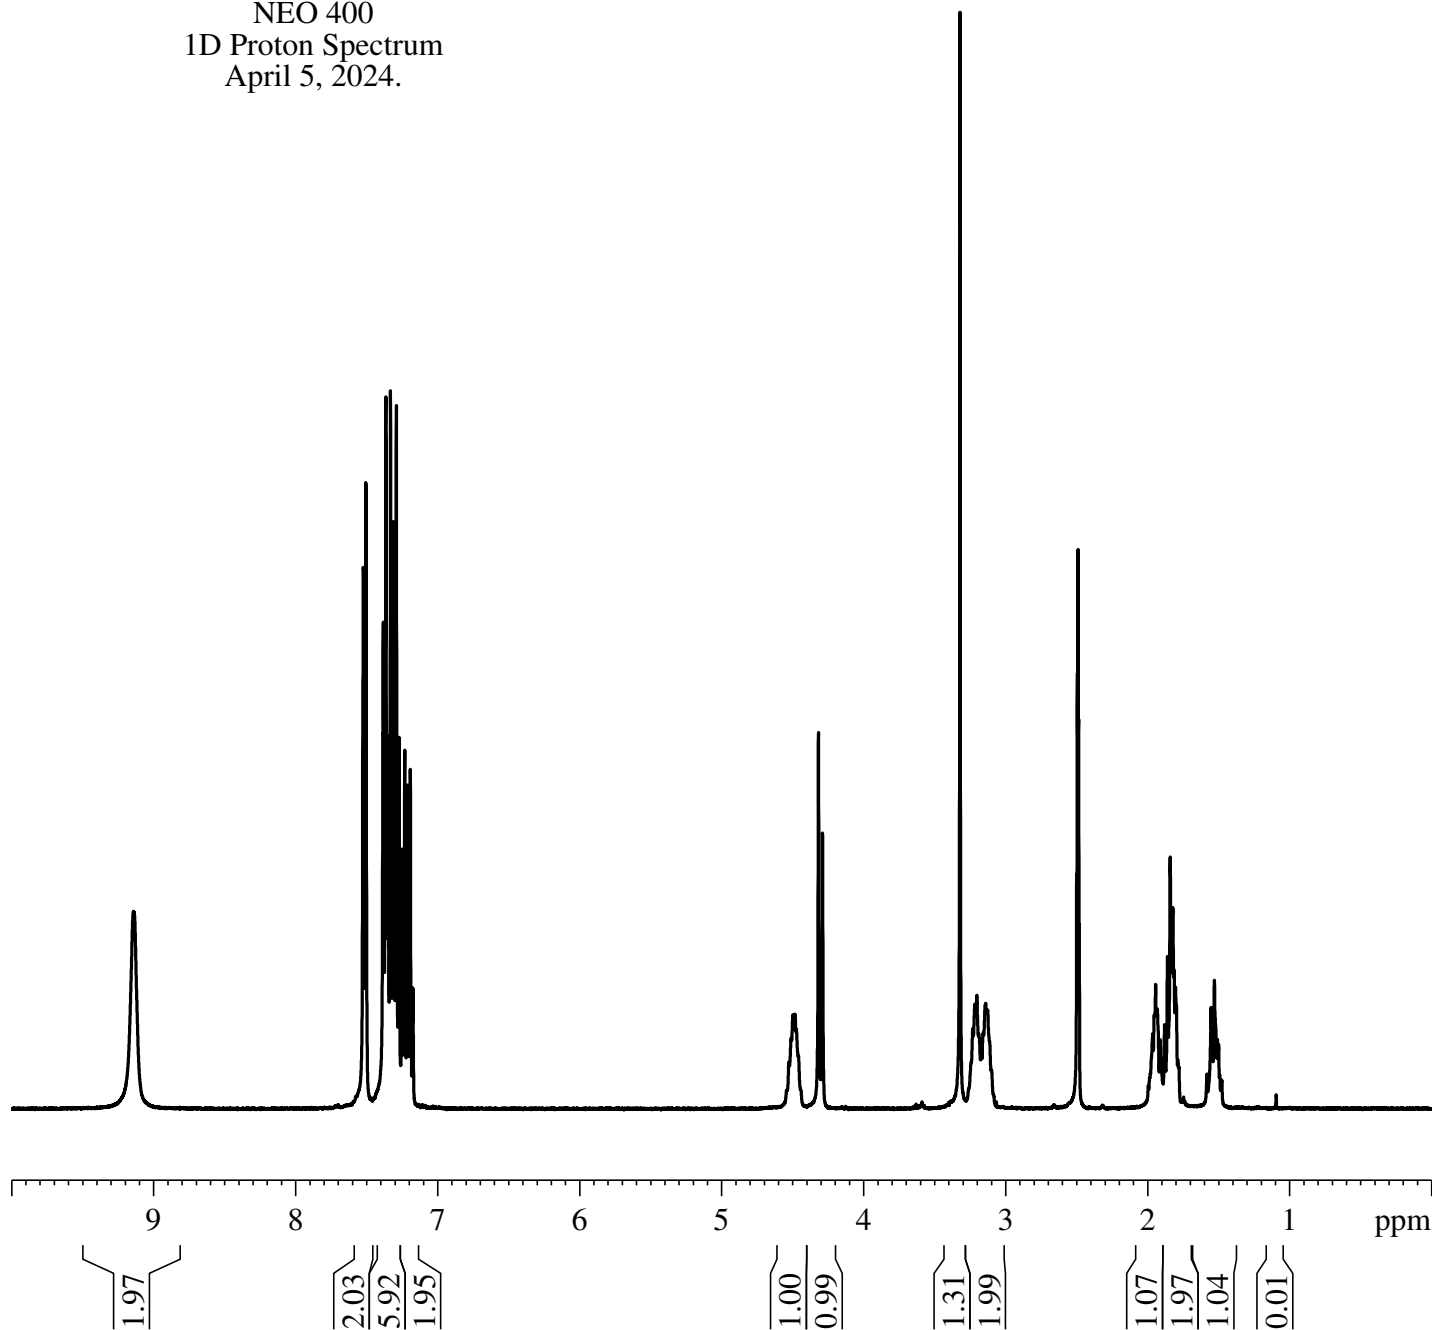

—9.141

Desoxy-D2FM HCl in DMSO-d6
NEO 400
1D Proton Spectrum
April 5, 2024.

7.523
7.505
7.386
7.383
7.365
7.350
7.332
7.312
7.291
7.271
7.250
7.231
7.213
7.211
7.192

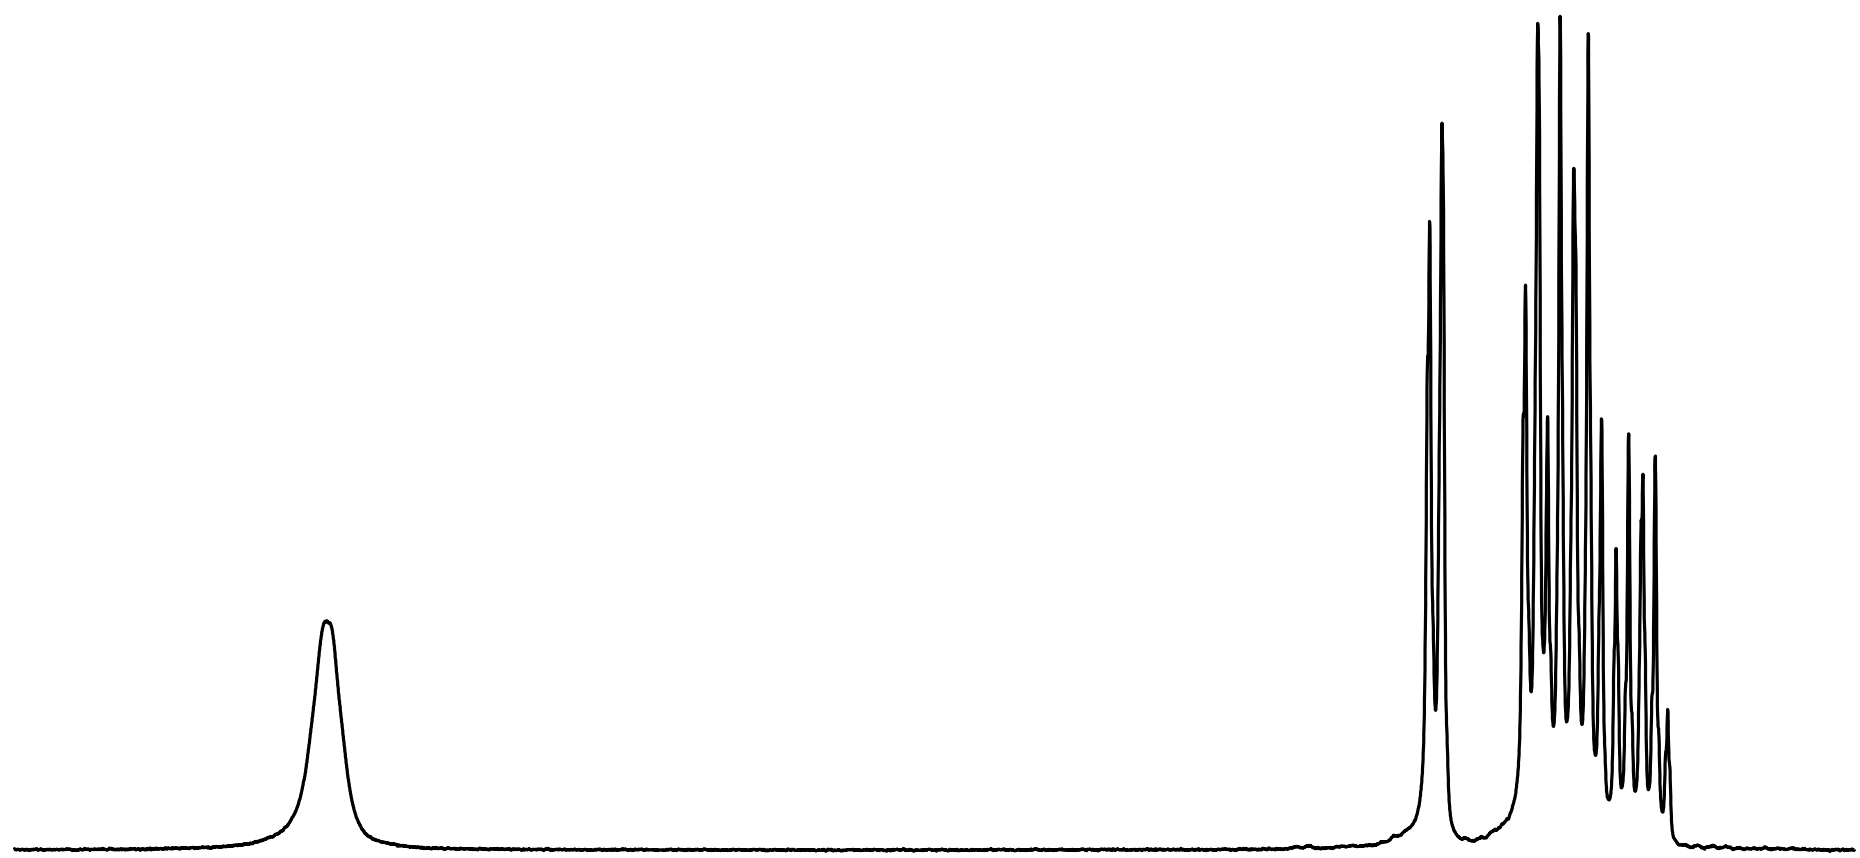

1.97

2.03

5.92

1.95

