


3-Fluorophenmetrazine HCl in DMSO-d6

Sample #2

NEO 400



1D Proton Spectrum

December 11, 2019.

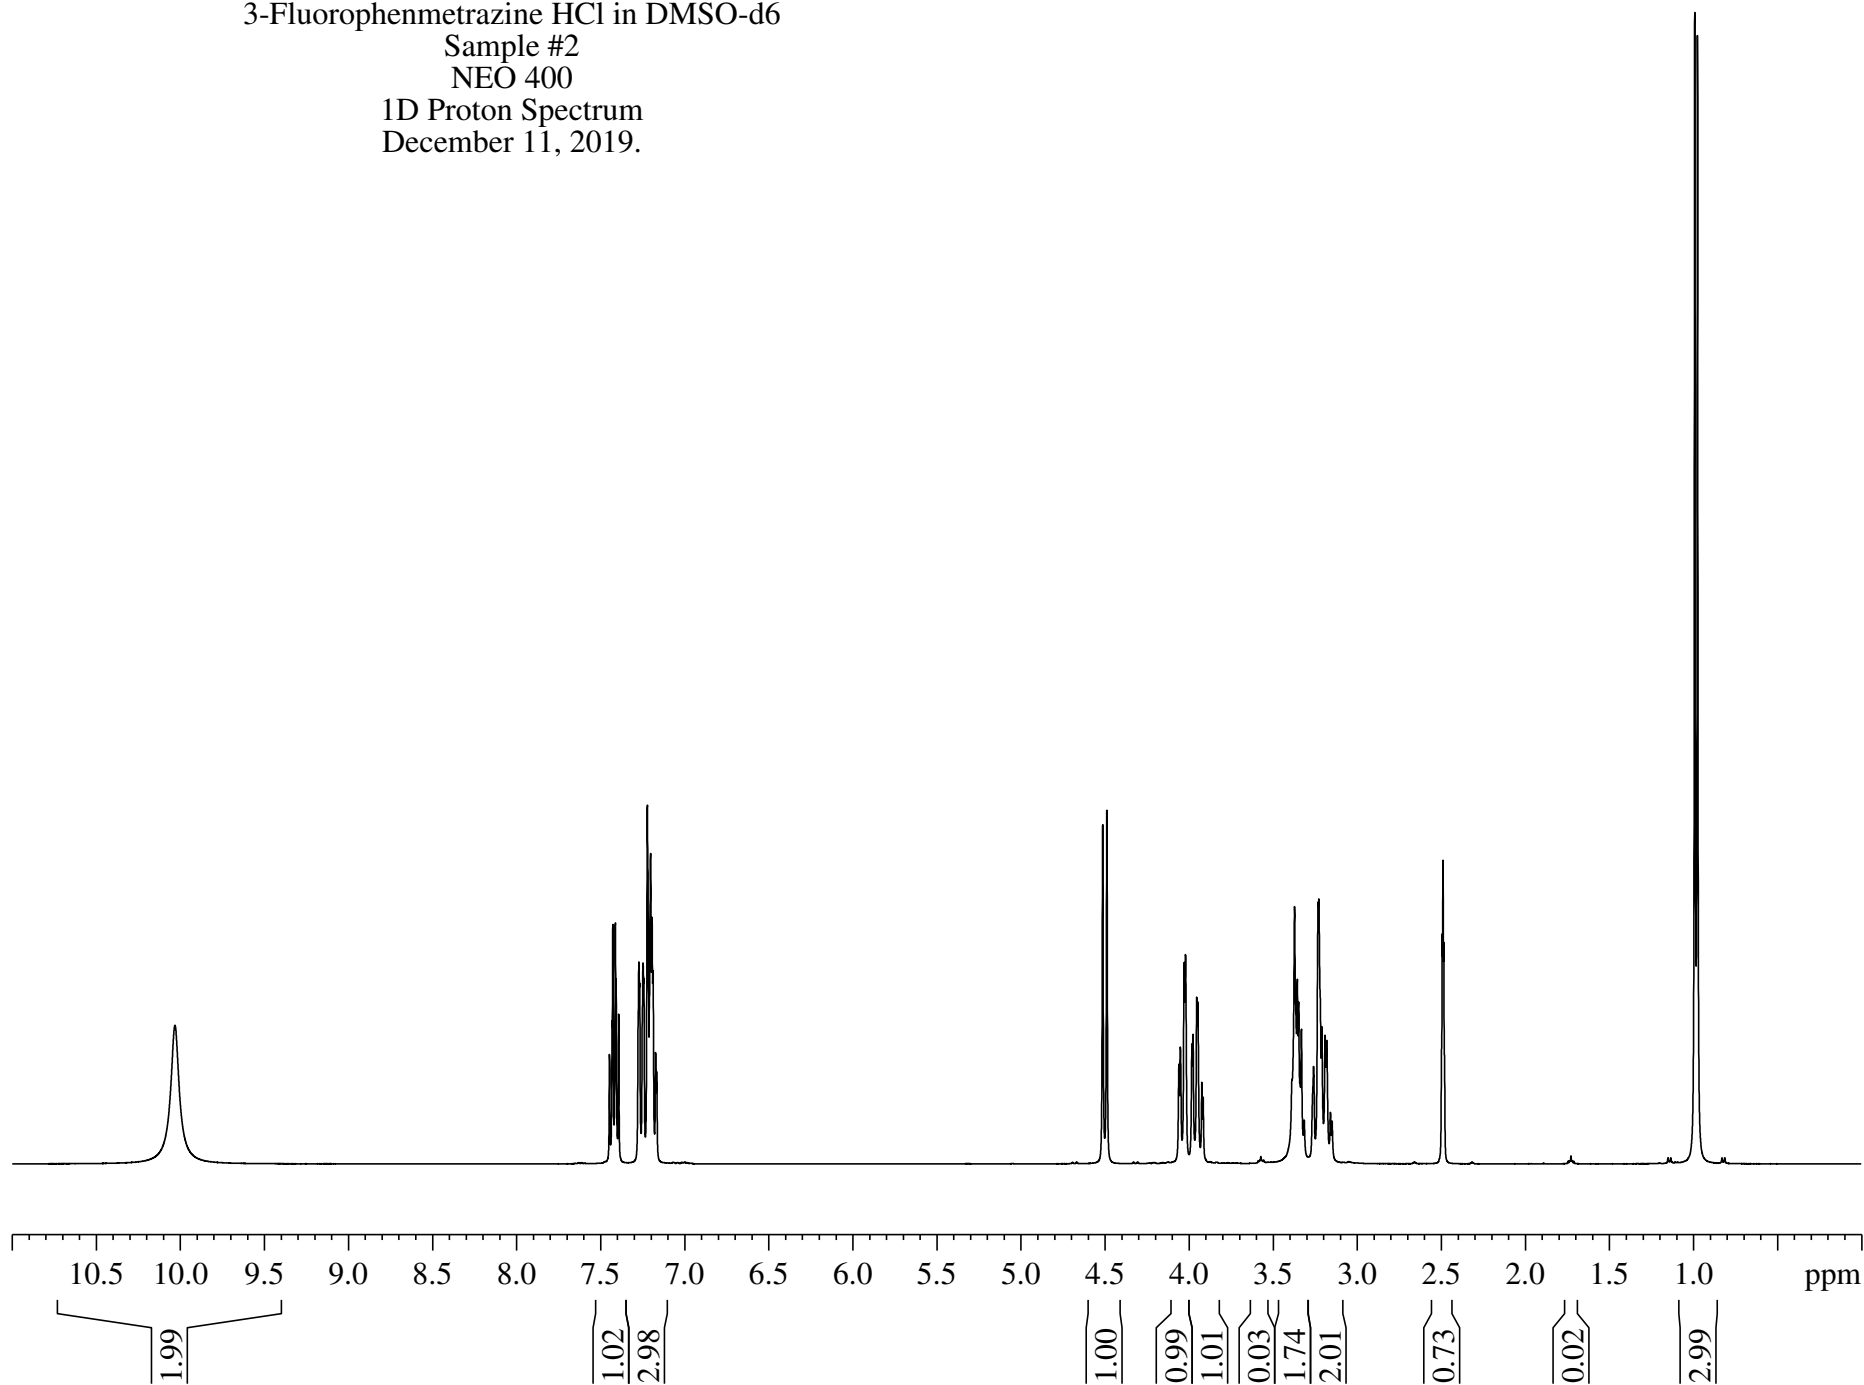

3-Fluorophenmetrazine HCl in DMSO-d6
Sample #2
NEO 400
1D Proton Spectrum
December 11, 2019.

— 10.03

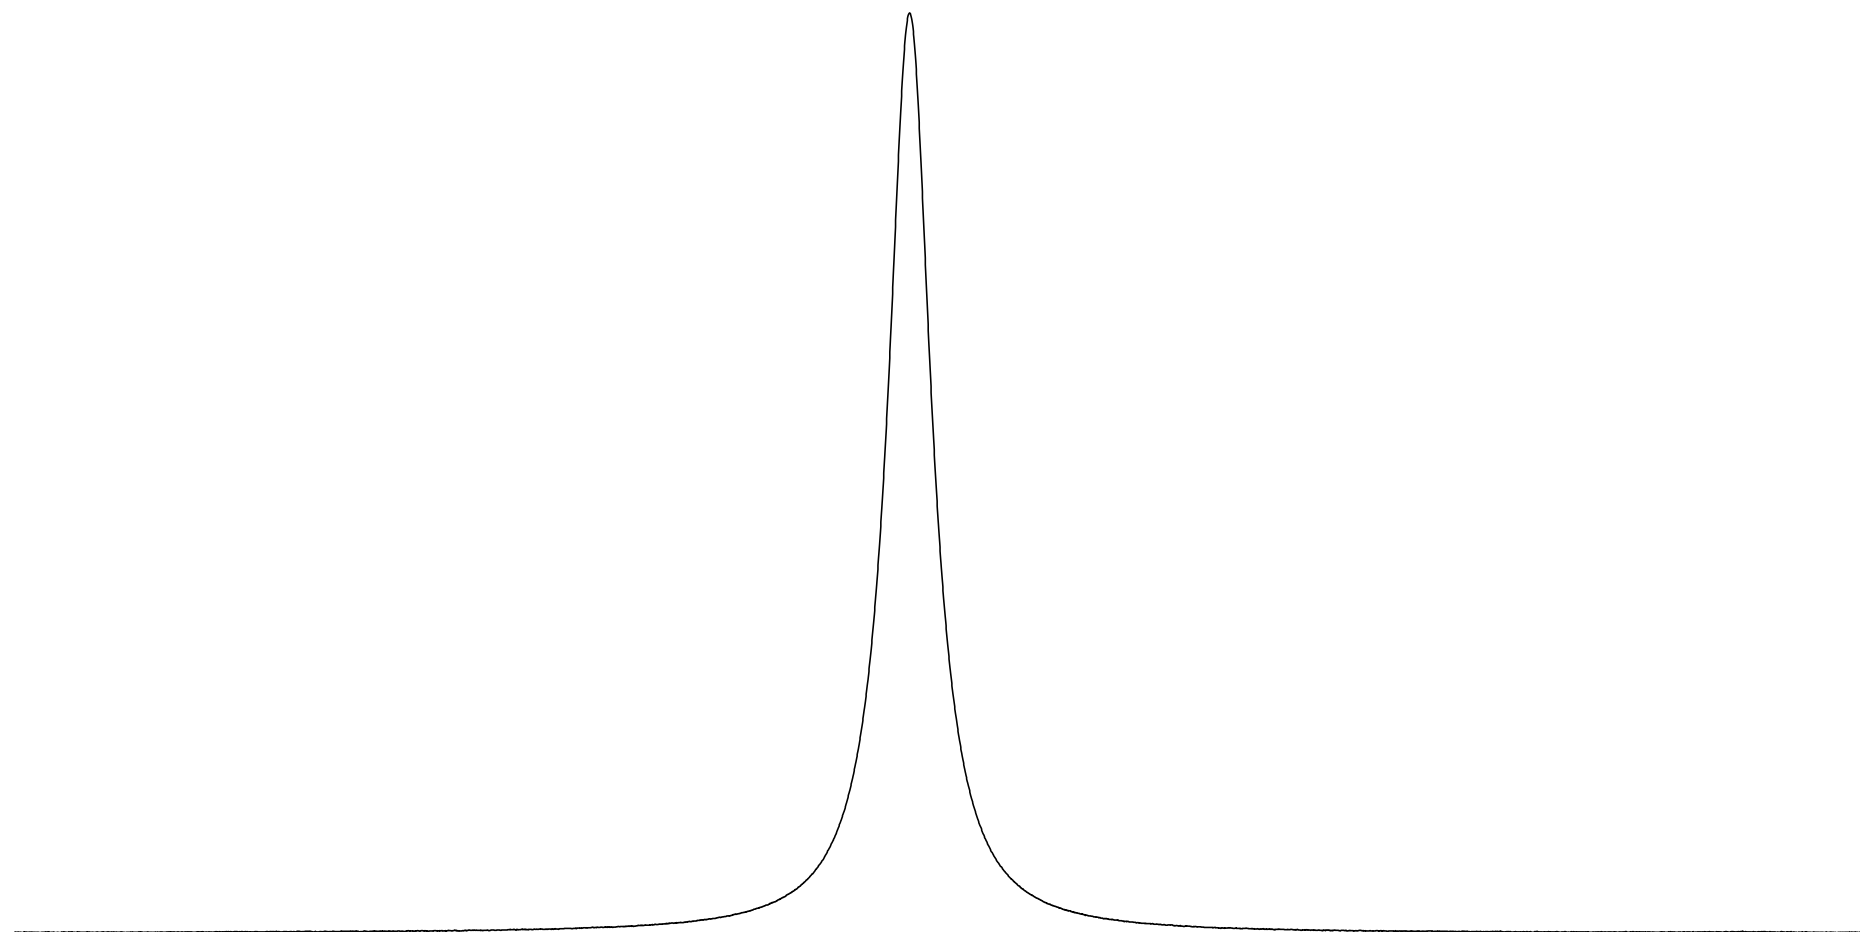


1.99



3-Fluorophenmetrazine HCl in DMSO-d6
Sample #2
NEO 400
1D Proton Spectrum
December 11, 2019.

7.45
7.43
7.43
7.41
7.41
7.39

7.27
7.27
7.25
7.24
7.22
7.20
7.19
7.19
7.17
7.17

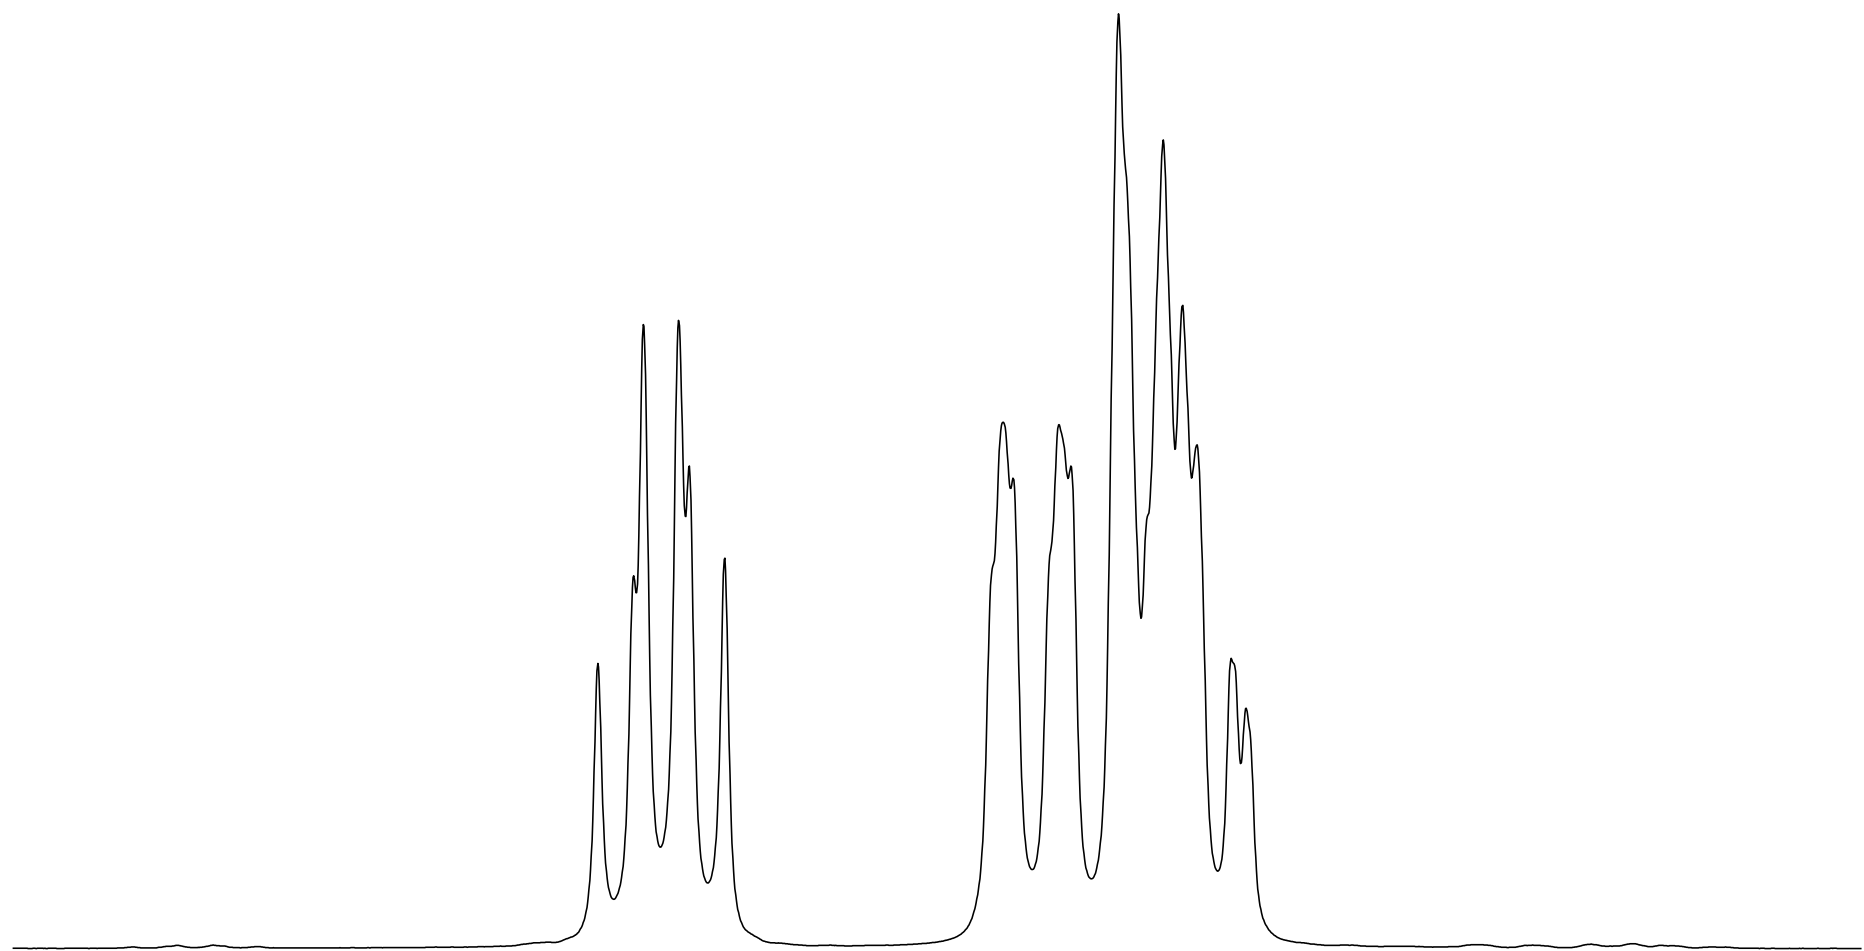


7.65 7.60 7.55 7.50 7.45 7.40 7.35 7.30 7.25 7.20 7.15 7.10 7.05 7.00 6.95 ppm

1.02

2.98

3-Fluorophenmetrazine HCl in DMSO-d6
Sample #2
NEO 400
1D Proton Spectrum
December 11, 2019.

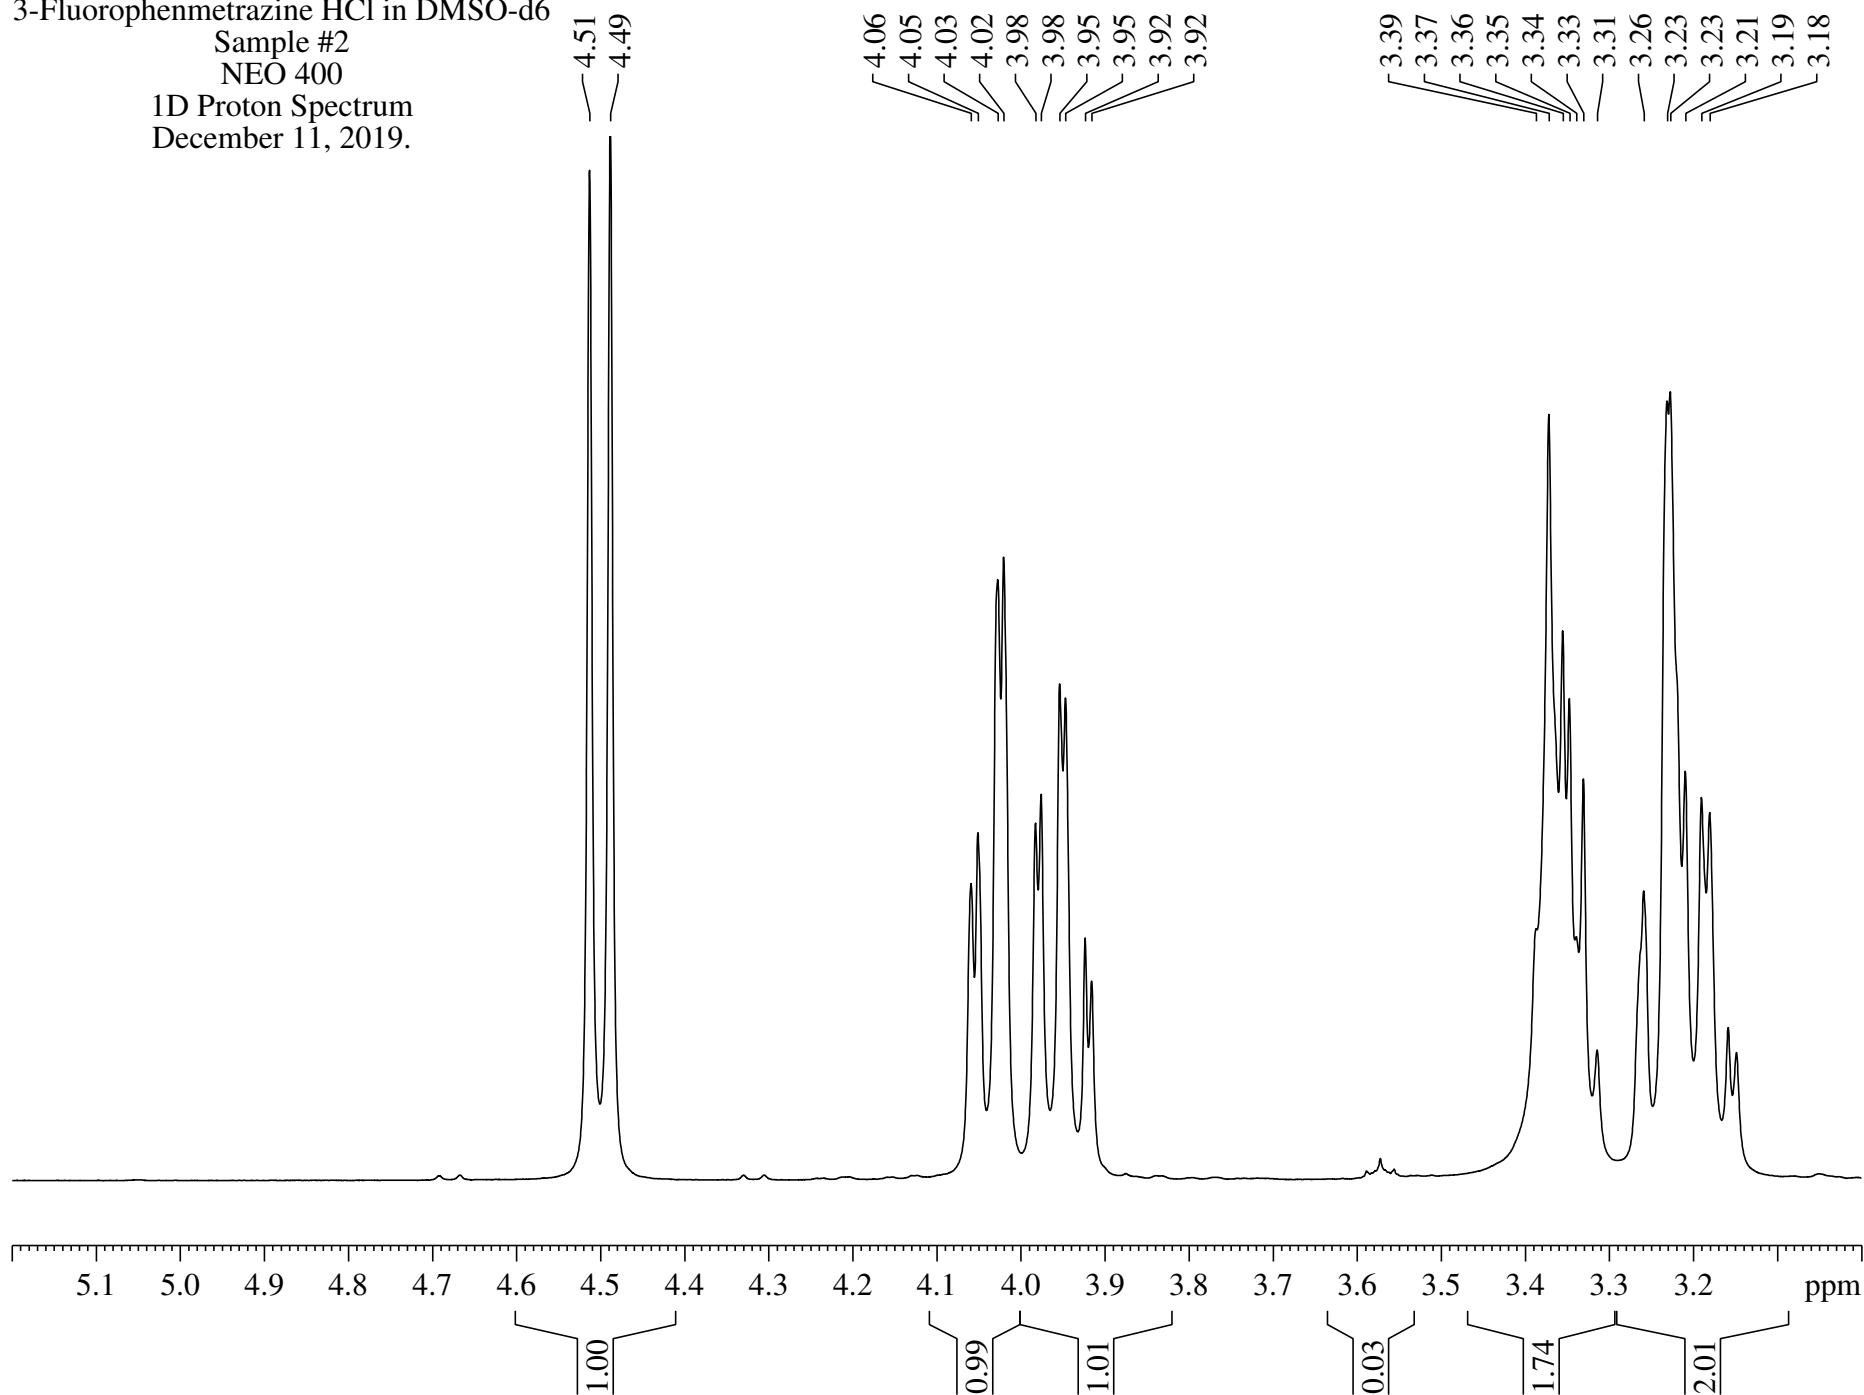


2.49
2.49
2.48

3-Fluorophenmetrazine HCl in DMSO-d6
Sample #2
NEO 400
1D Proton Spectrum
December 11, 2019.

1.73

0.99
0.97

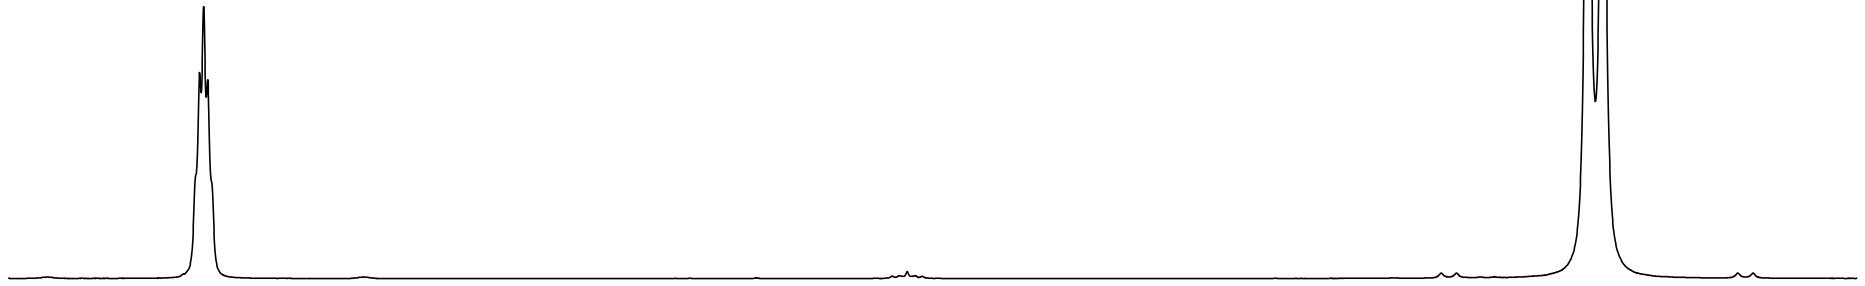

2.6 2.5 2.4 2.3 2.2 2.1 2.0 1.9 1.8 1.7 1.6 1.5 1.4 1.3 1.2 1.1 1.0 0.9 0.8 ppm

0.73

0.02

2.99