


l-Benzyl-4-methylpiperazine HCl in DMSO-d₆
Sample 2
NEO 400
1D Proton Spectrum
June 2, 2021.

Current Data Parameters
NAME Syntharise060221
EXPNO 450
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210602
Time 9.34 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 (zg30)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 295.2 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters
SI 65536
SF 400.3400072 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

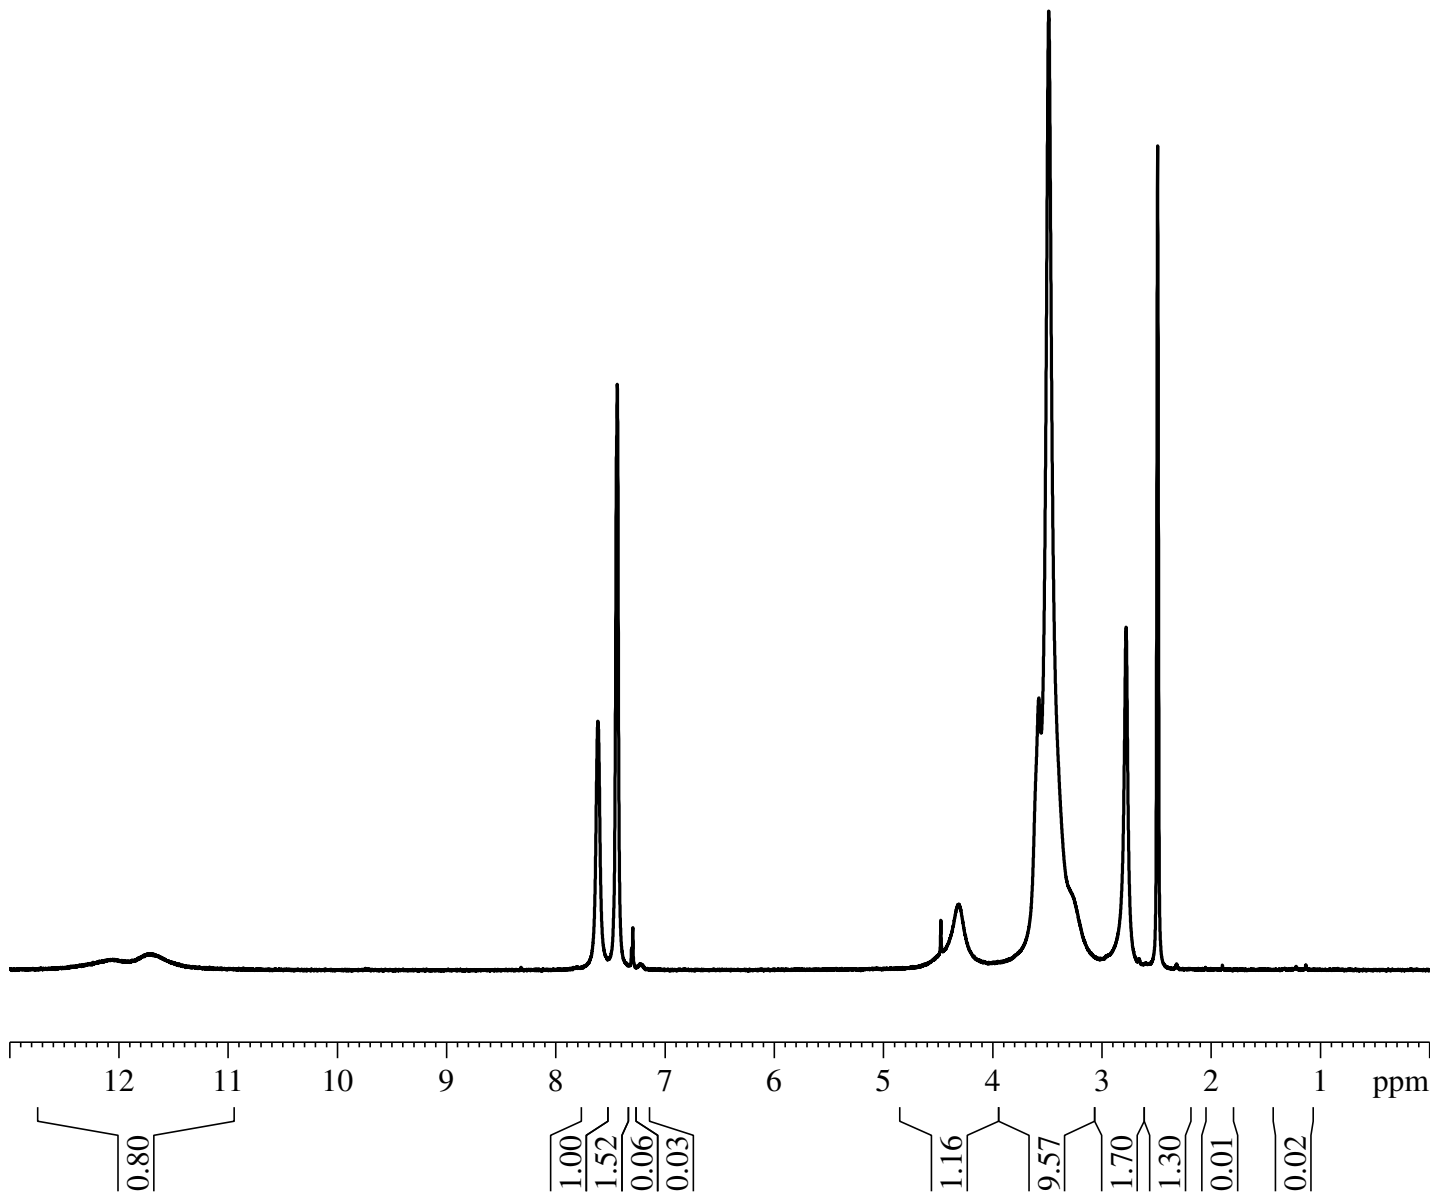

l-Benzyl-4-methylpiperazine HCl in DMSO-d₆
Sample 2
NEO 400
1D Proton Spectrum
June 2, 2021.


— 12.064

— 11.725

— 7.613

— 7.437

— 7.294

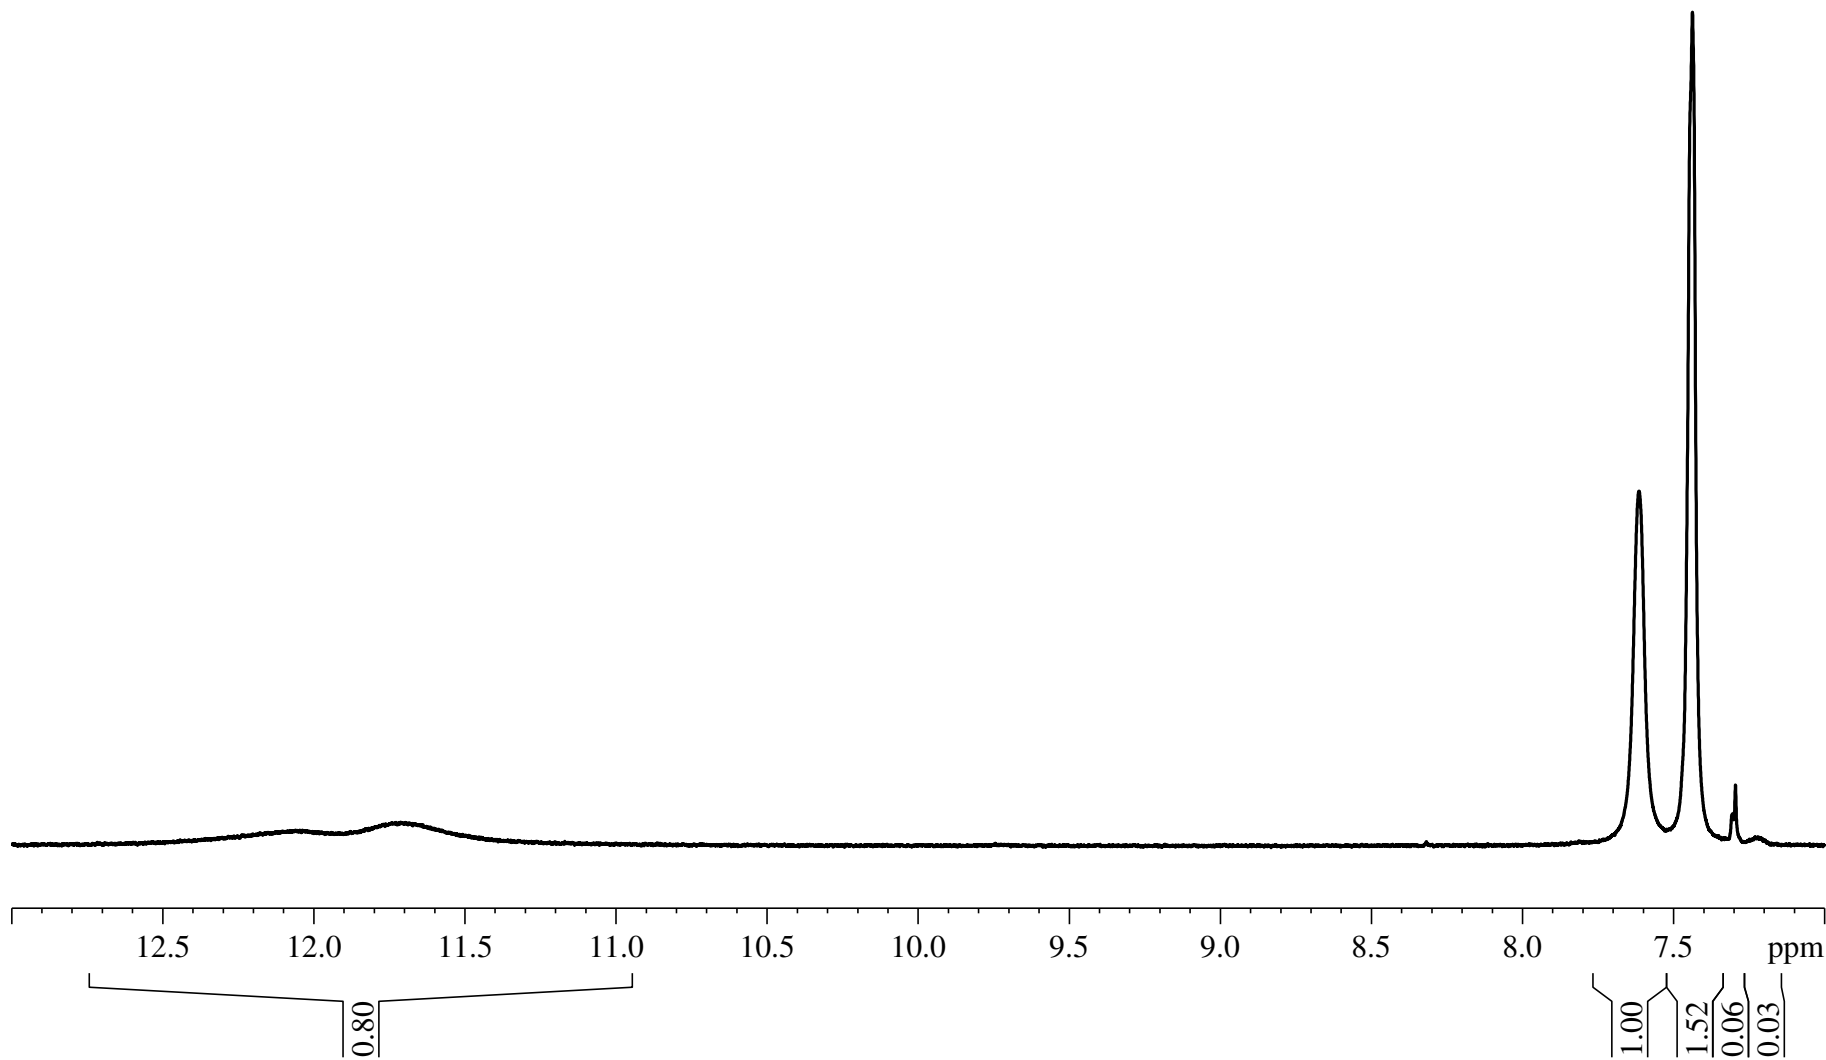

l-Benzyl-4-methylpiperazine HCl in DMSO-d6
Sample 2
NEO 400
1D Proton Spectrum
June 2, 2021.

