
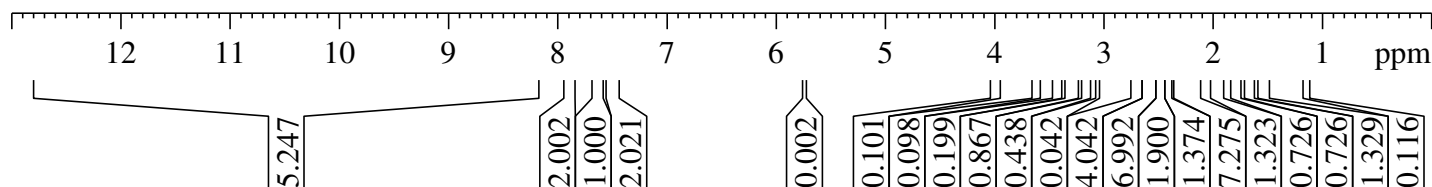


4-MAB in DMSO-d6  
NEO 400  
1D Proton Spectrum  
November 11, 2022.

Current Data Parameters  
NAME Syntharise111122  
EXPNO 400  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20221111  
Time 14.22 h  
INSTRUM Avance Neo 400  
PROBHD Z104450\_0313 (  
PULPROG zg30  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 0  
SWH 8196.722 Hz  
FIDRES 0.250144 Hz  
AQ 3.9976959 sec  
RG 101  
DW 61.000 usec  
DE 13.54 usec  
TE 295.6 K  
D1 0.10000000 sec  
TD0 1  
SFO1 400.3424721 MHz  
NUC1 1H  
P0 3.33 usec  
P1 10.00 usec  
PLW1 14.20300007 W

F2 - Processing parameters  
SI 65536  
SF 400.3400072 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

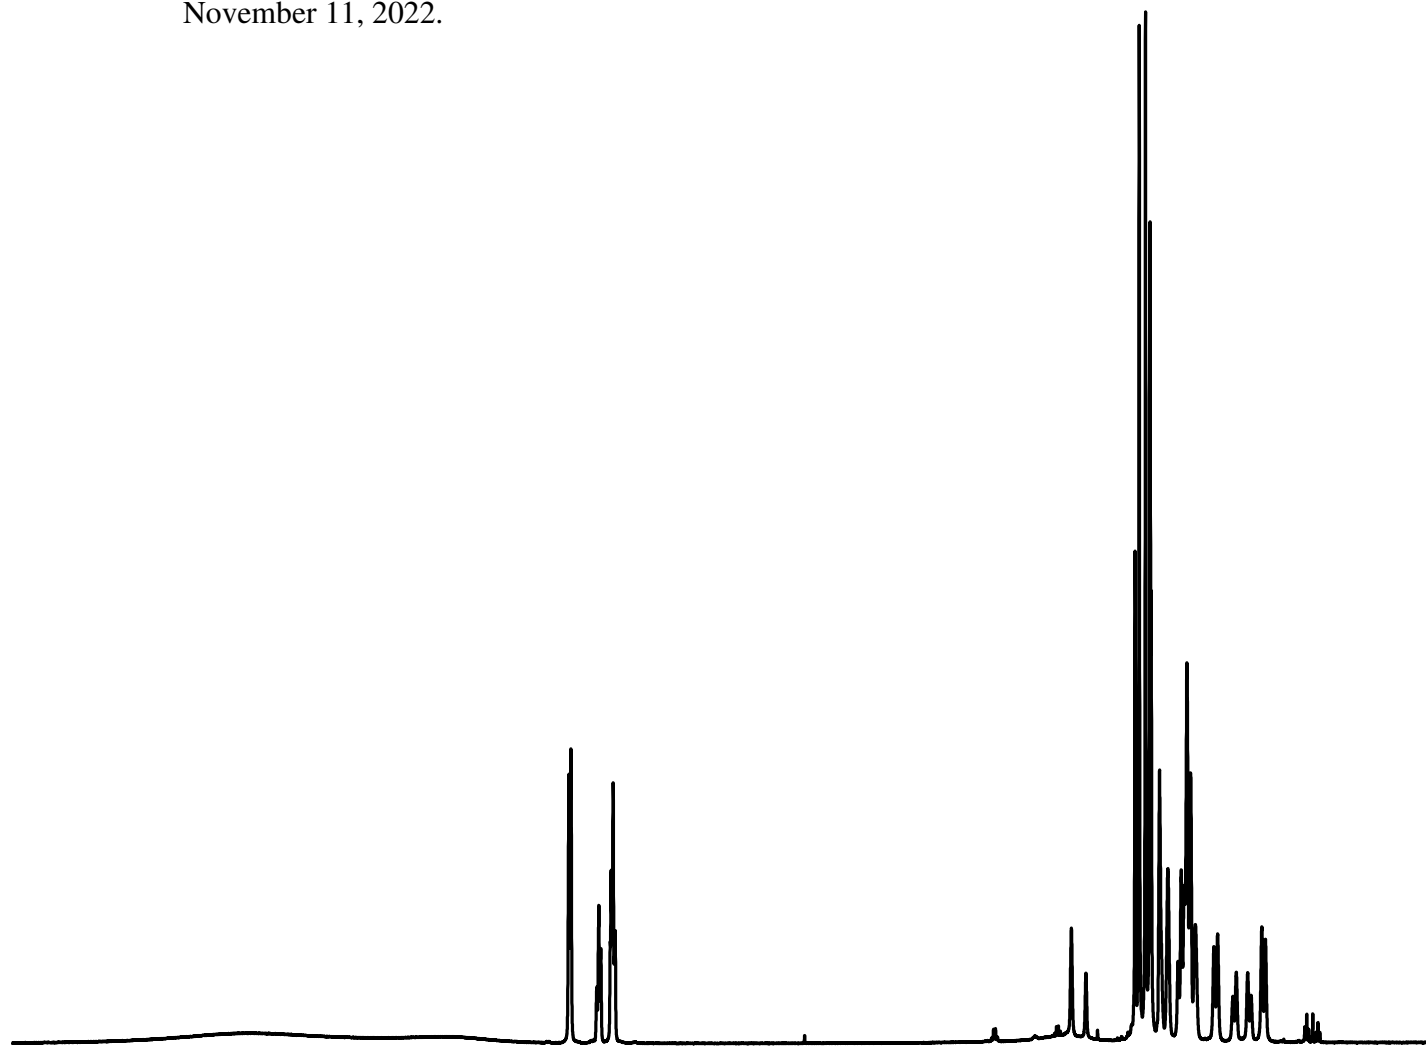


4-MAB in DMSO-d6  
NEO 400  
1D Proton Spectrum  
November 11, 2022.

— 10.812

— 9.013

7.898  
7.879  
7.624  
7.606  
7.520  
7.512  
7.500  
7.493  
7.482  
7.474

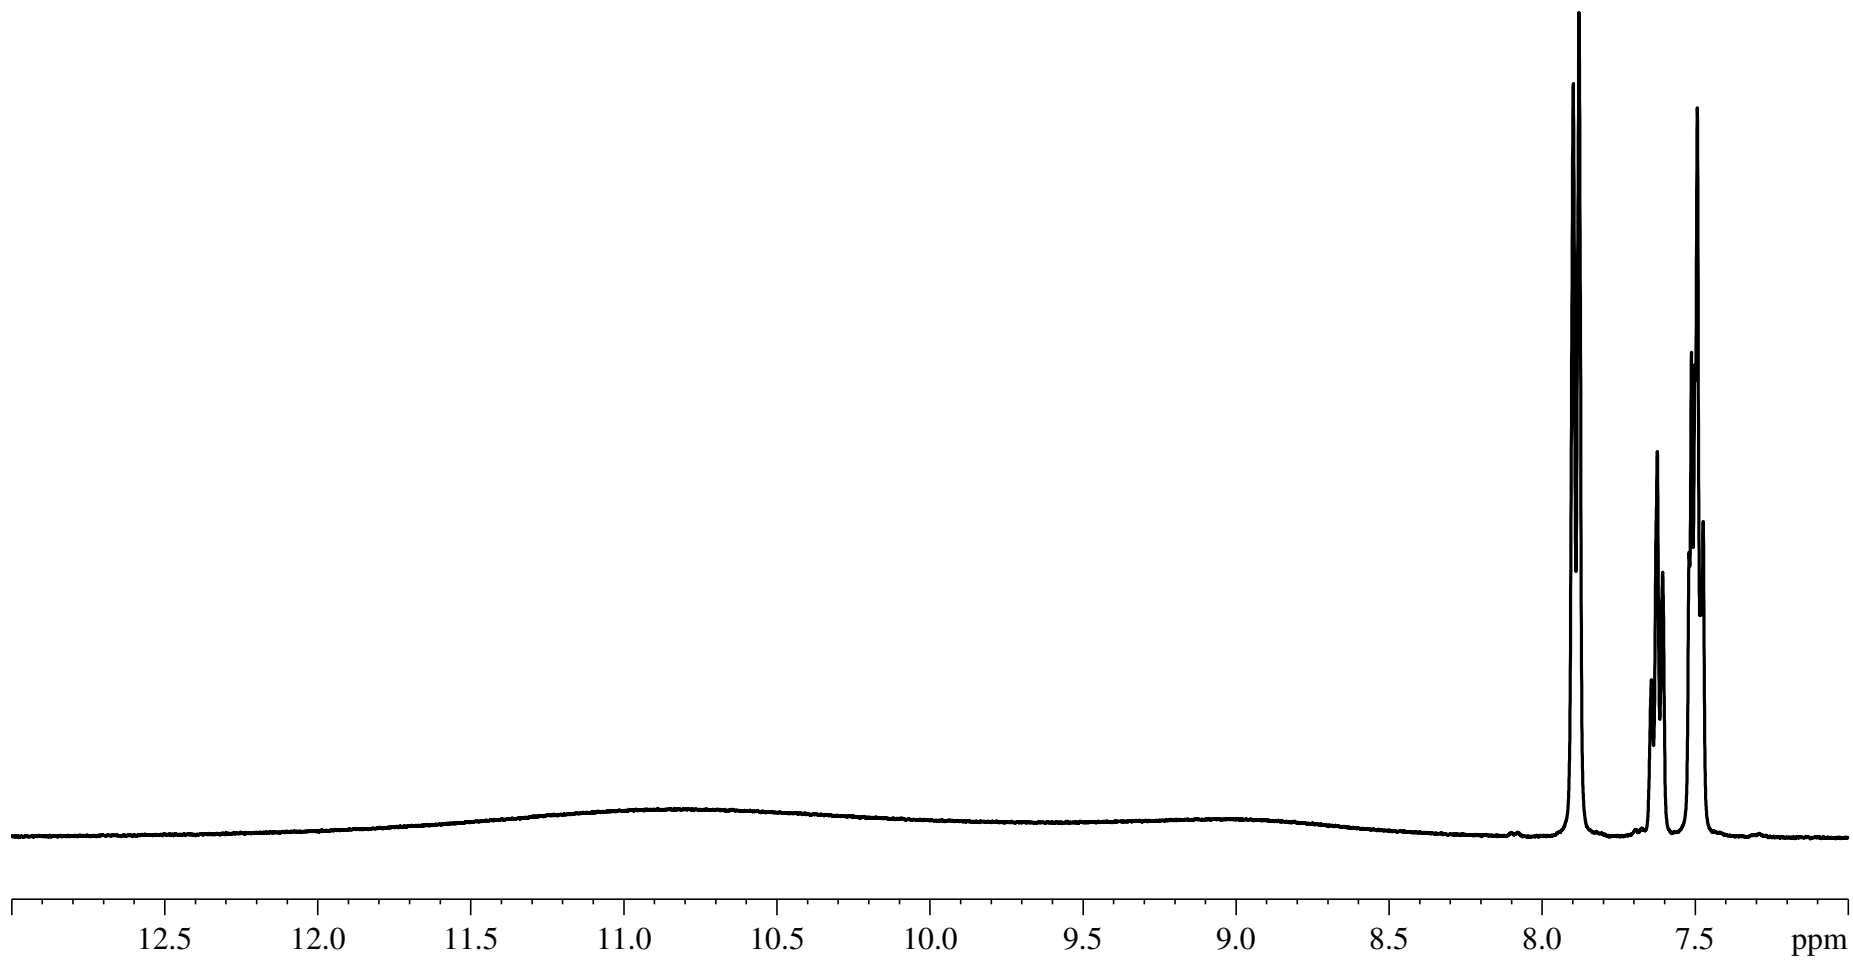


5.247

2.002

1.000

2.021

4-MAB in DMSO-d6  
NEO 400  
1D Proton Spectrum  
November 11, 2022.

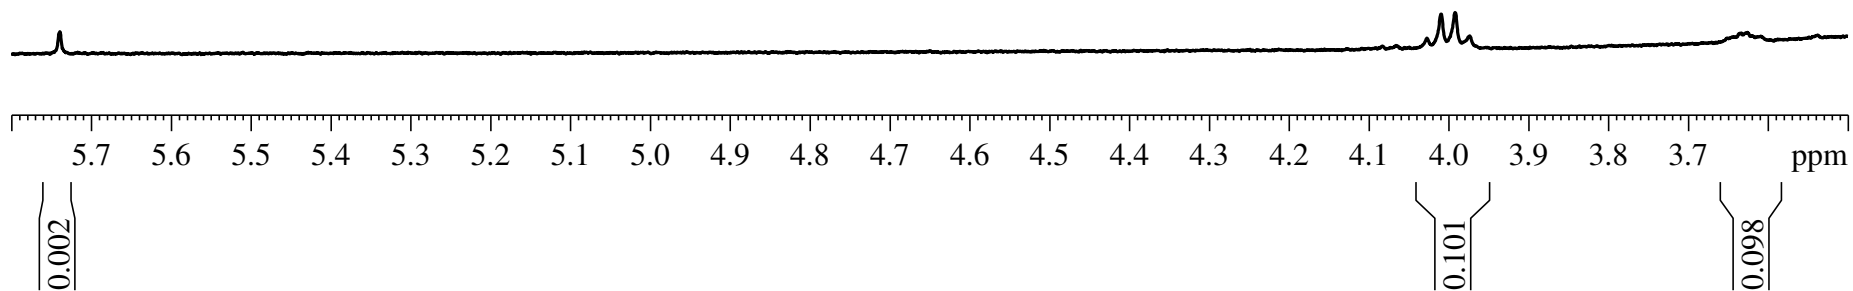

4-MAB in DMSO-d6  
NEO 400  
1D Proton Spectrum  
November 11, 2022.

