


MPPB HCl in DMSO-d6
NEO 400
1D Proton Spectrum
January 6, 2023.

Current Data Parameters
NAME Syntharise010623
EXPNO 400
PROCNO 1


F2 - Acquisition Parameters
Date_ 20230106
Time 12.35 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 ()
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 297.1 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters
SI 65536
SF 400.3400072 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

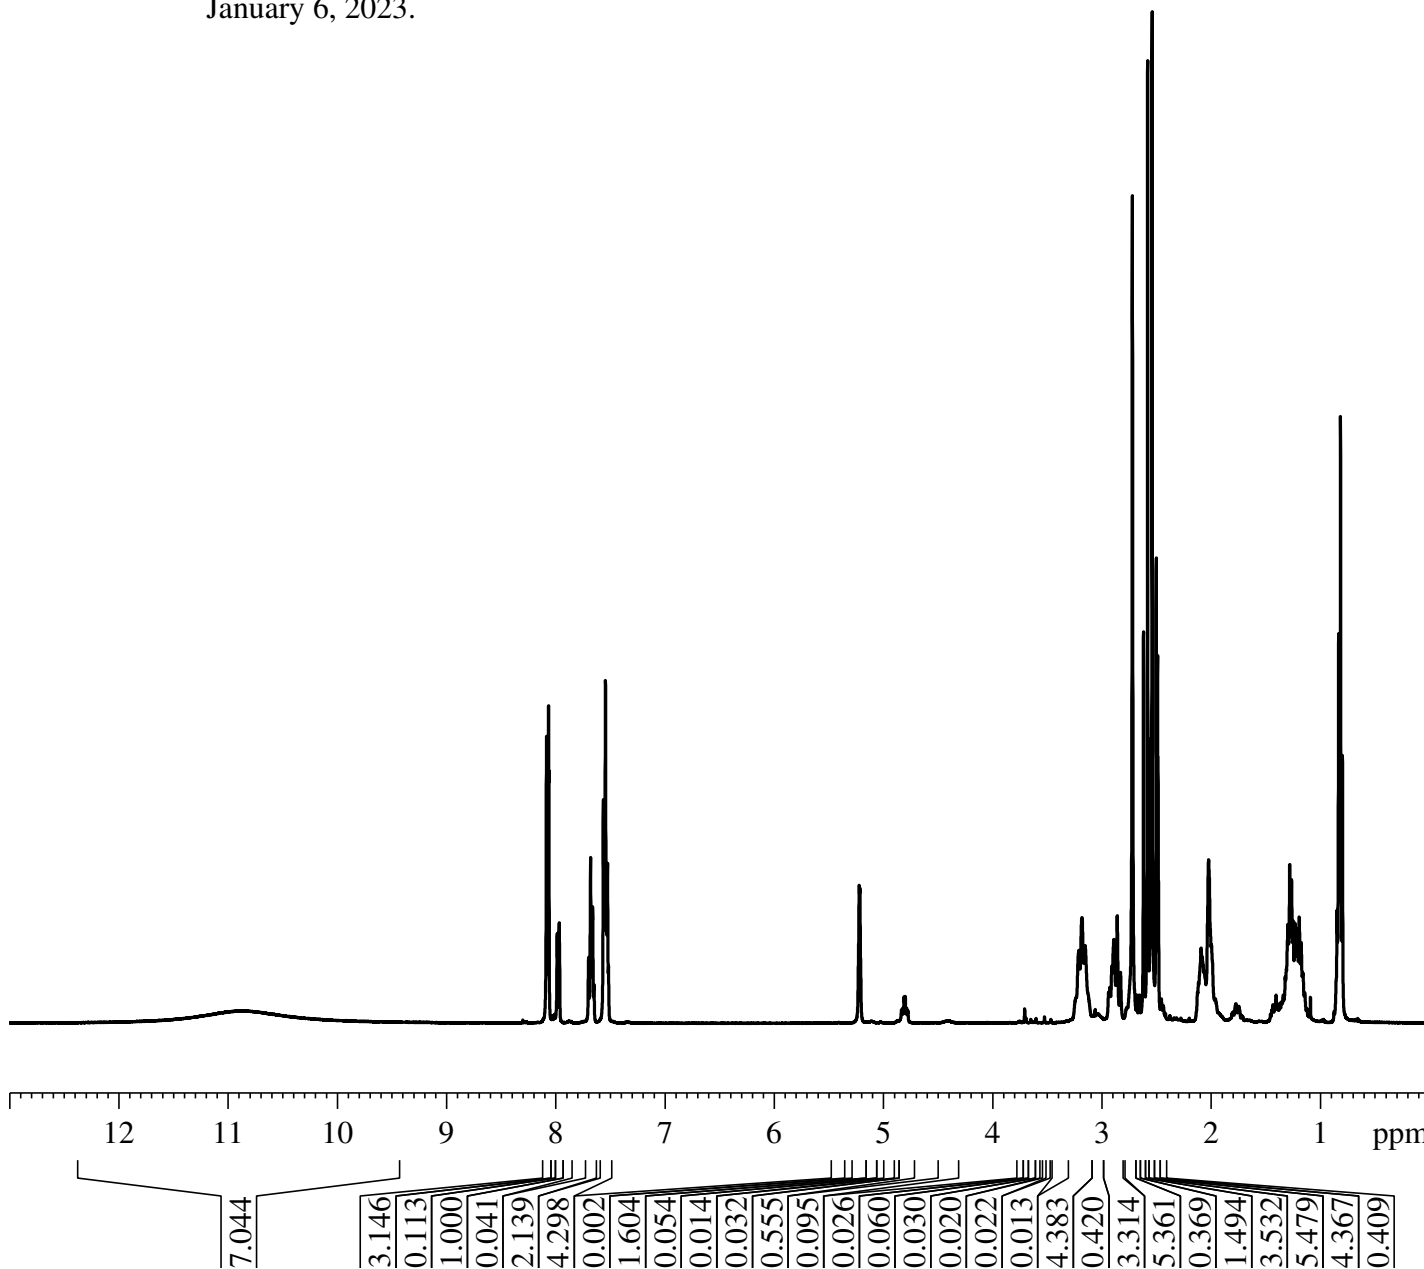

MPPB HCl in DMSO-d6
NEO 400
1D Proton Spectrum
January 6, 2023.

— 10.876

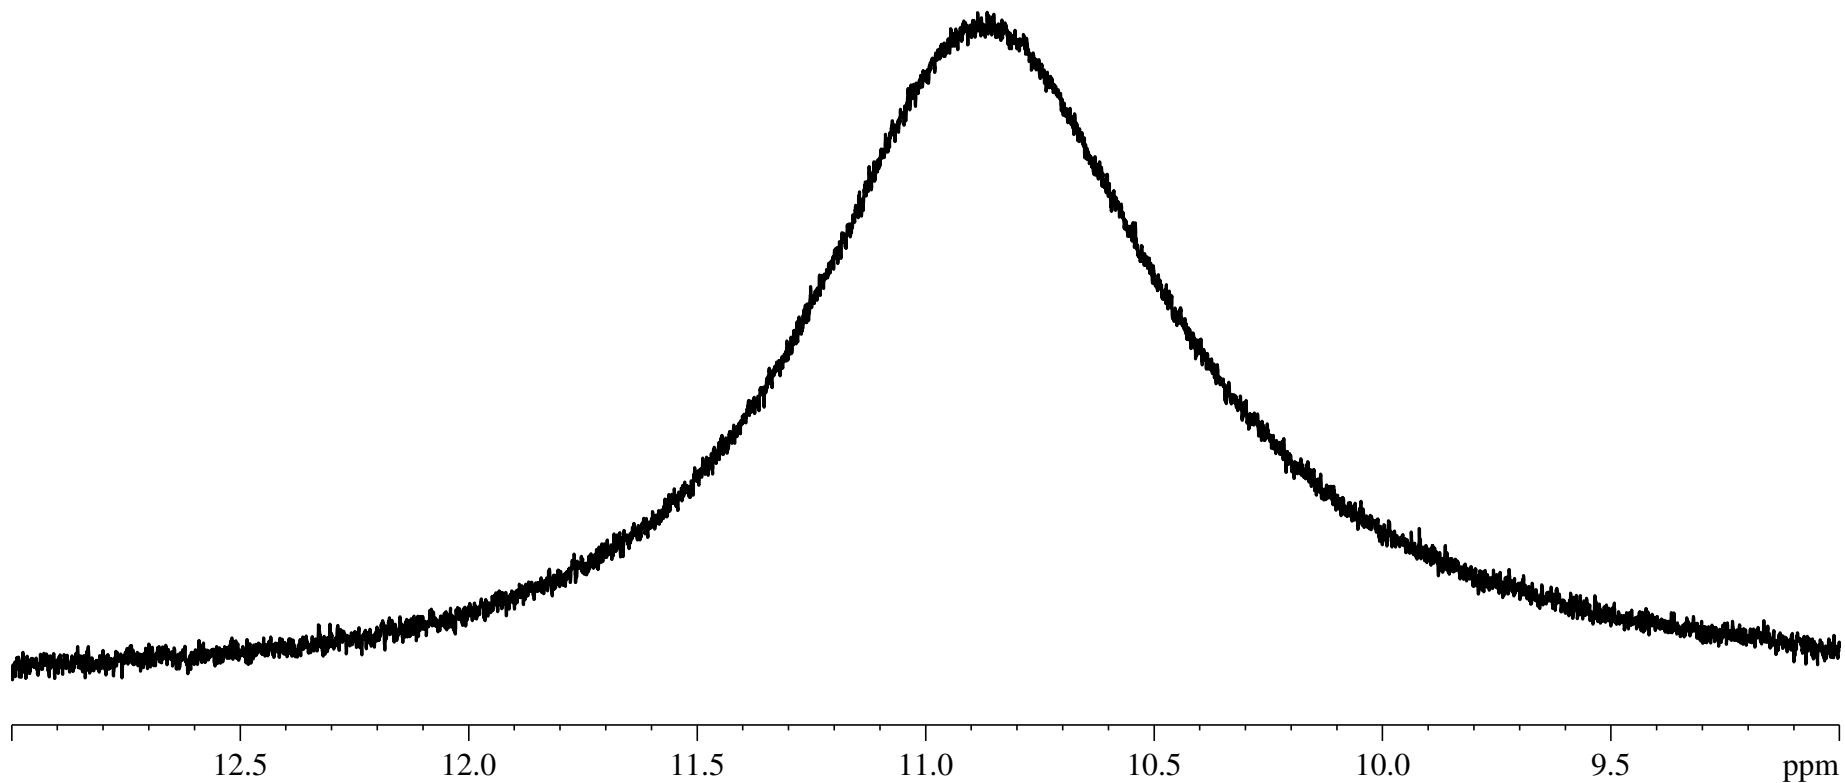


7.044

MPPB HCl in DMSO-d6
NEO 400
1D Proton Spectrum
January 6, 2023.

8.084
8.066
8.063
7.986
7.968

7.681

7.564
7.545
7.526

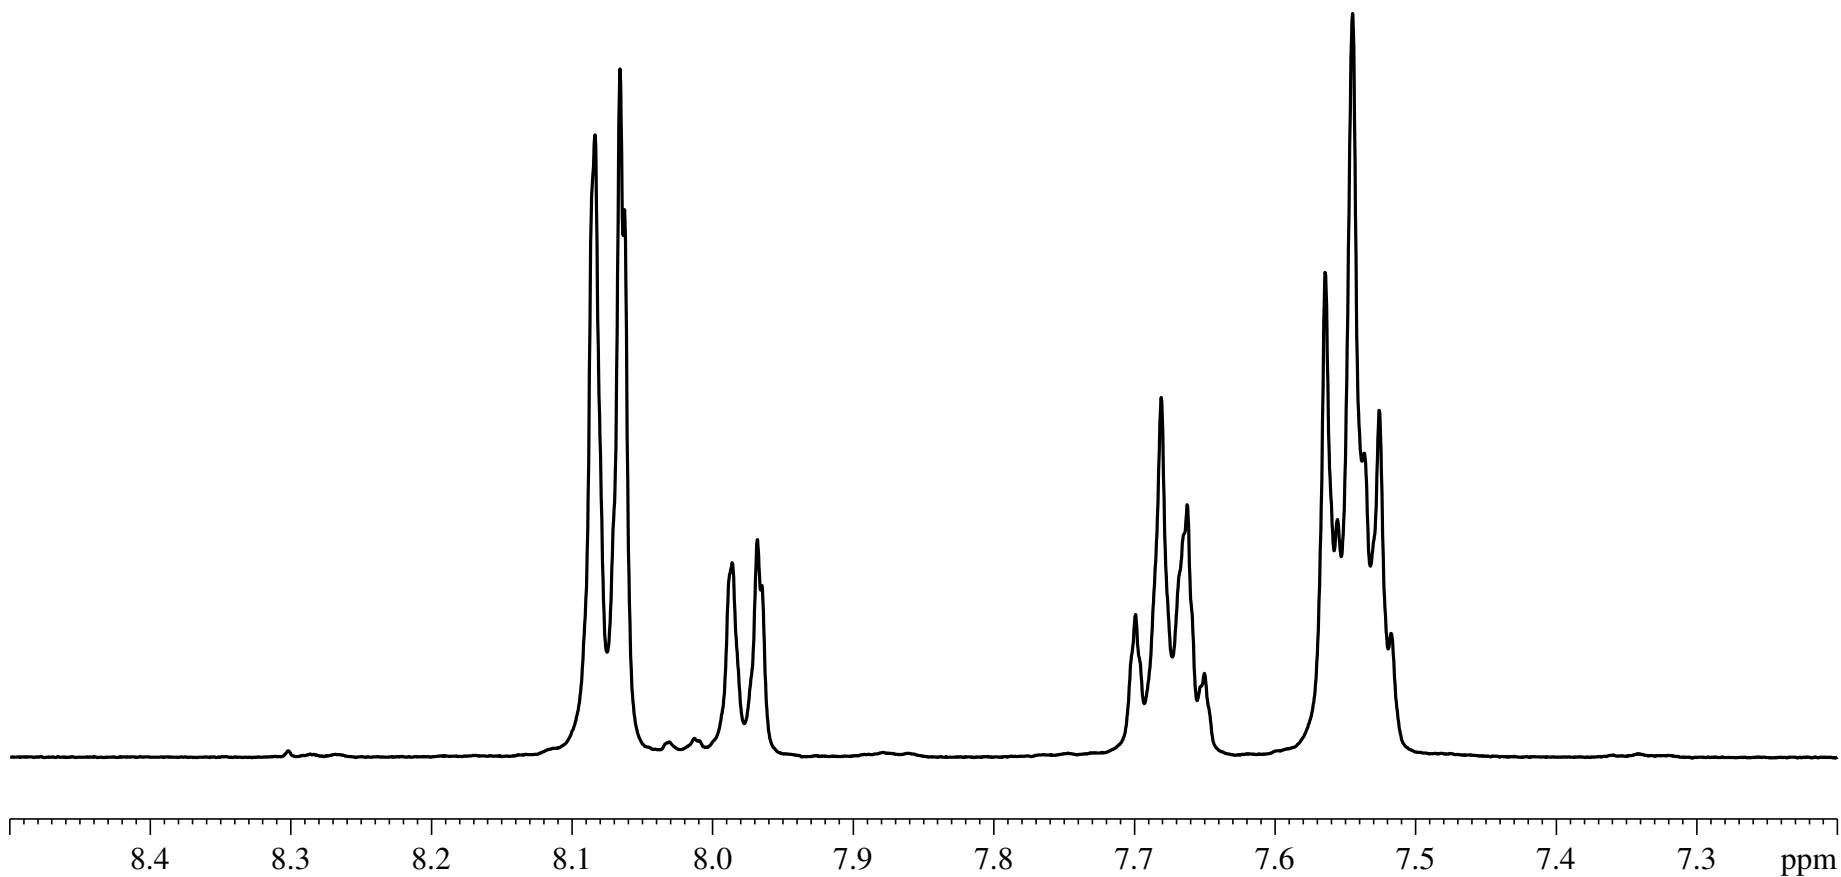



3.146
0.113
1.000
0.041

2.139

4.298

MPPB HCl in DMSO-d6
NEO 400
1D Proton Spectrum
January 6, 2023.

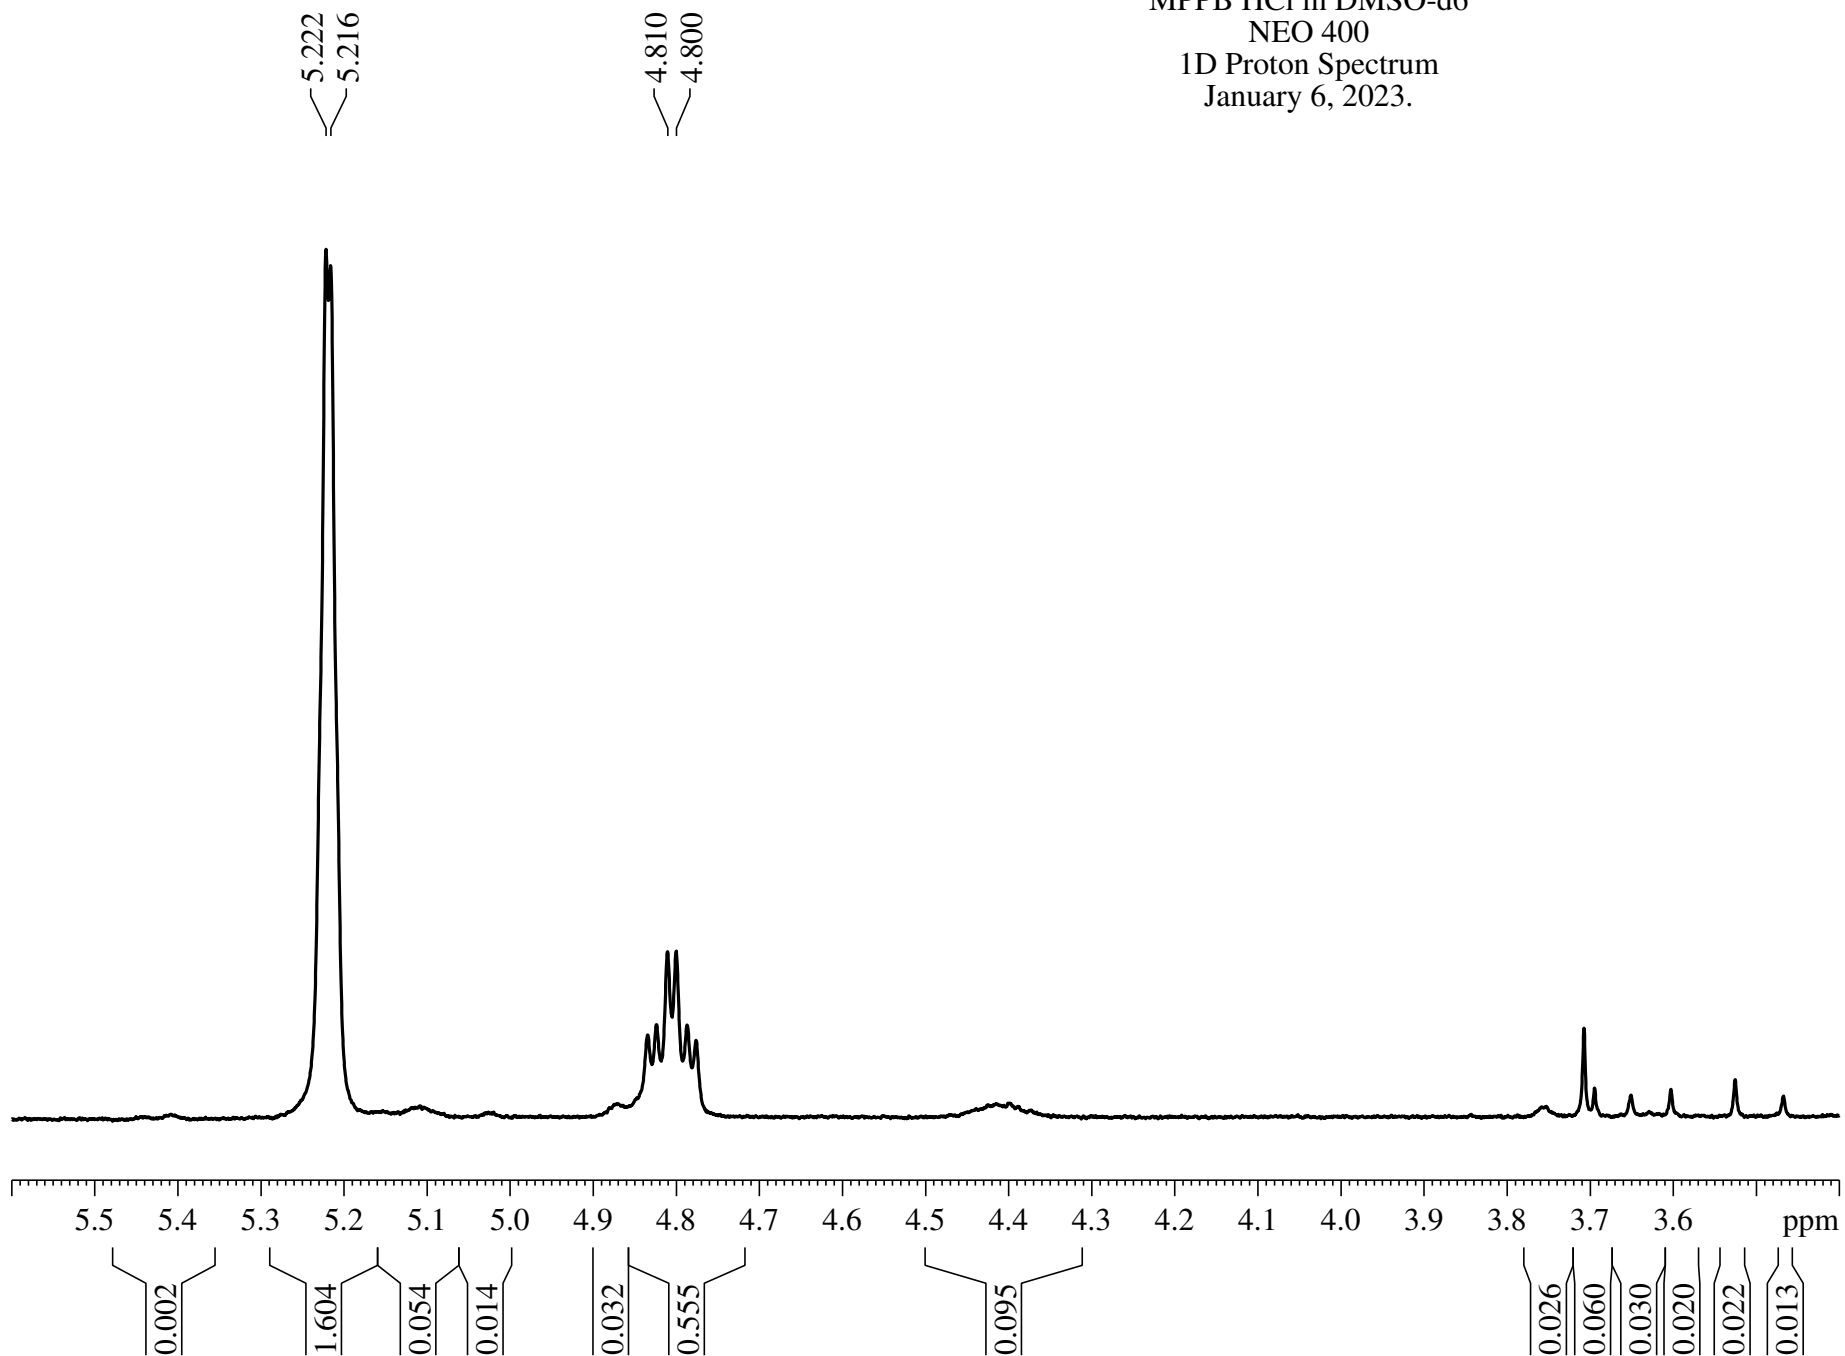


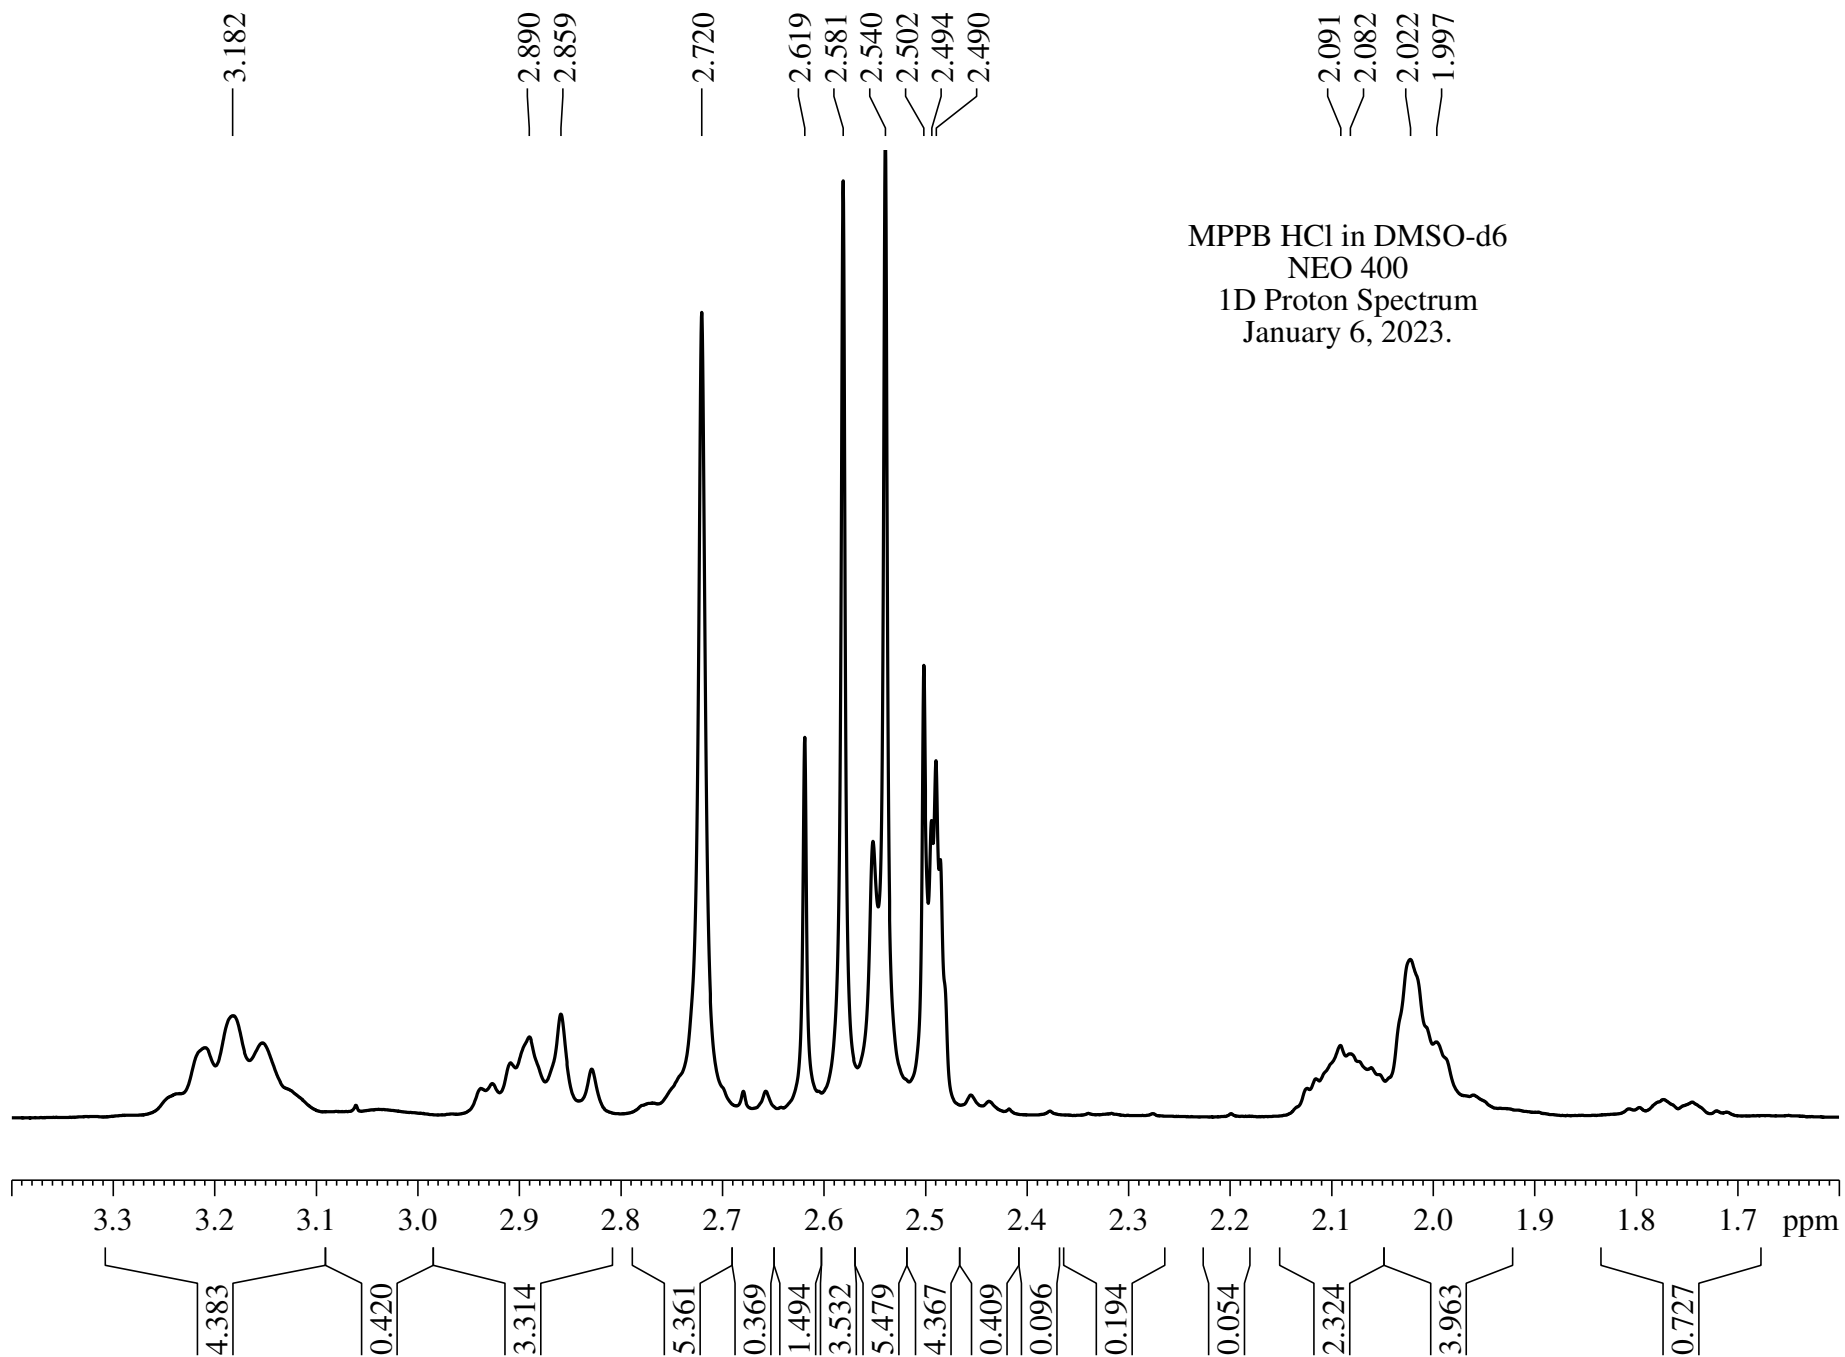

MPPB HCl in DMSO-d6
NEO 400
1D Proton Spectrum
January 6, 2023.

— 1.280
— 1.263

— 0.831
— 0.815
— 0.797

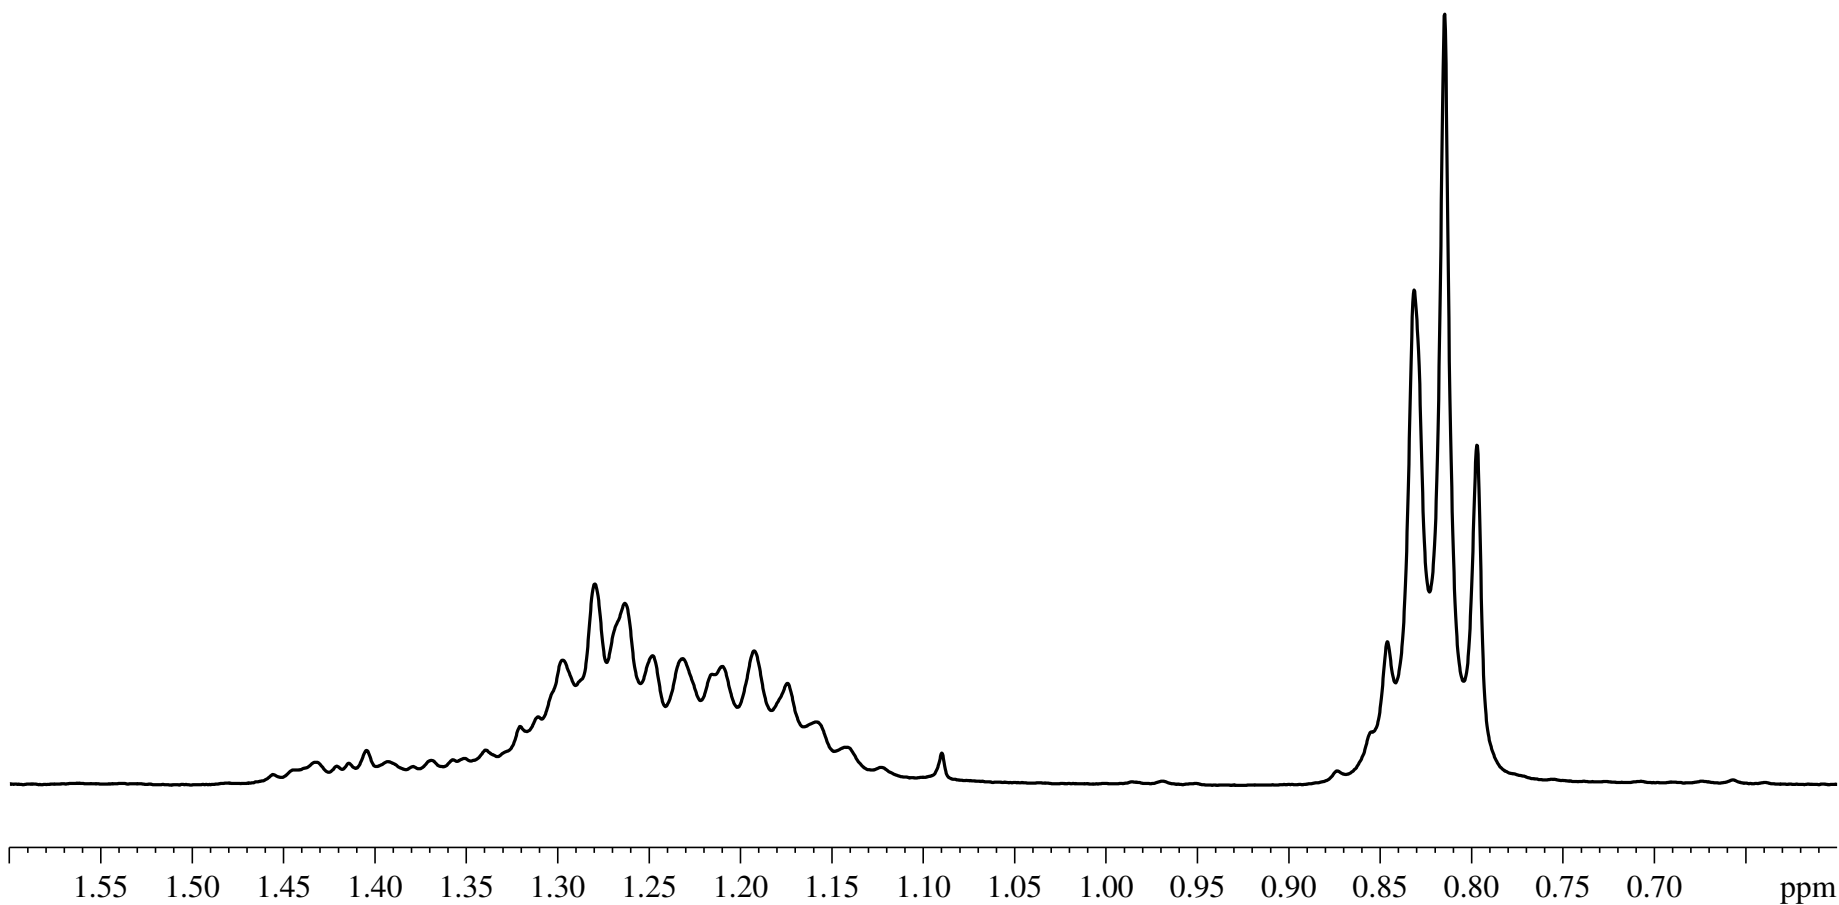

1.114

8.211

0.149

6.961