



4-PrO-DMT in DMSO-d6
NEO 400
1D Proton Spectrum
August 22, 2023.

Current Data Parameters
NAME Syntharise082223
EXPNO 410
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230822
Time 13.37 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 (zg30)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 296.3 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W



F2 - Processing parameters
SI 65536
SF 400.340068 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

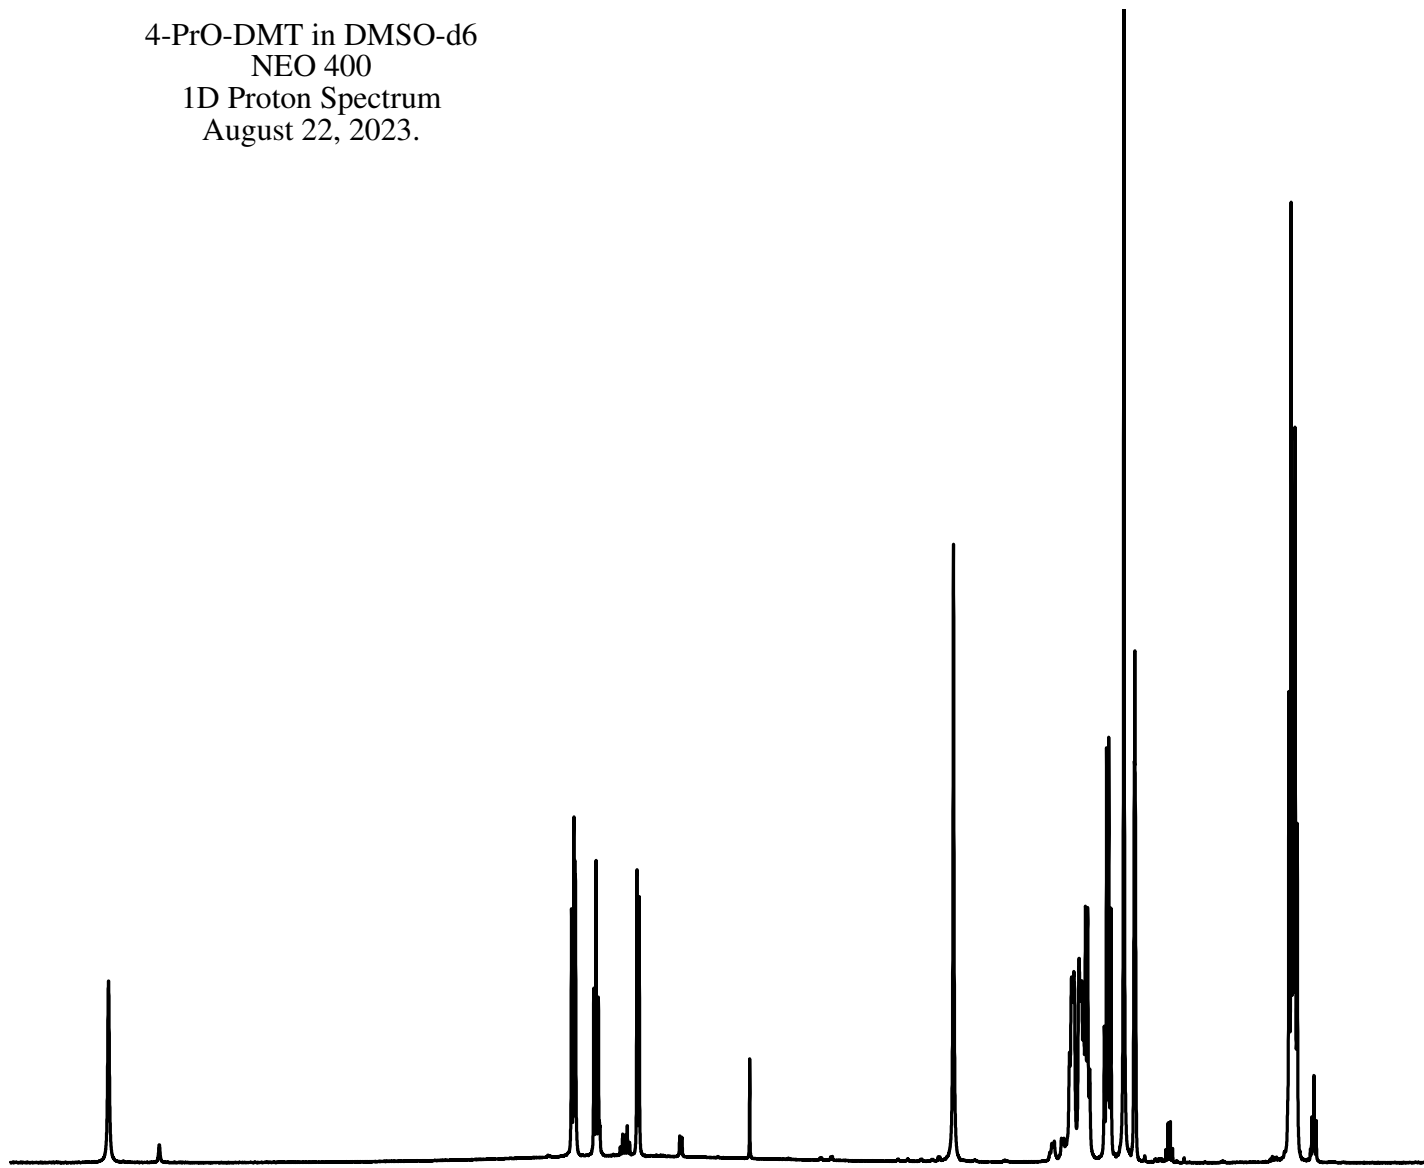


1.00
0.08

2.27
1.36
0.38
1.24
0.27
0.22
0.05
0.05
0.03
0.02
0.02
0.02
0.04
2.06
0.03
0.02
0.23
0.27
2.18
4.15
2.43
3.08
1.98
0.05
0.15
0.07


4-PrO-DMT in DMSO-d6
NEO 400
1D Proton Spectrum
August 22, 2023.

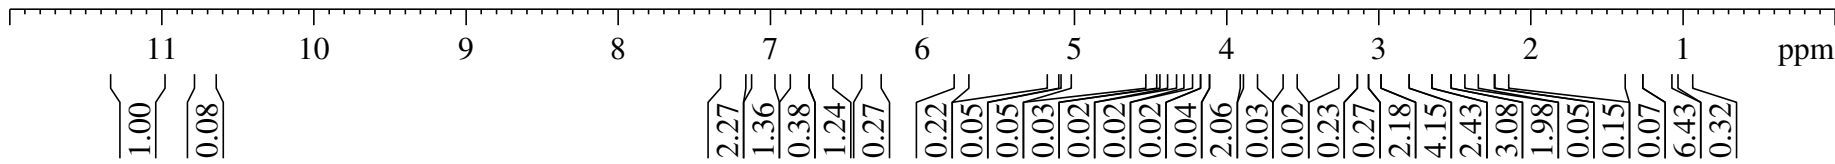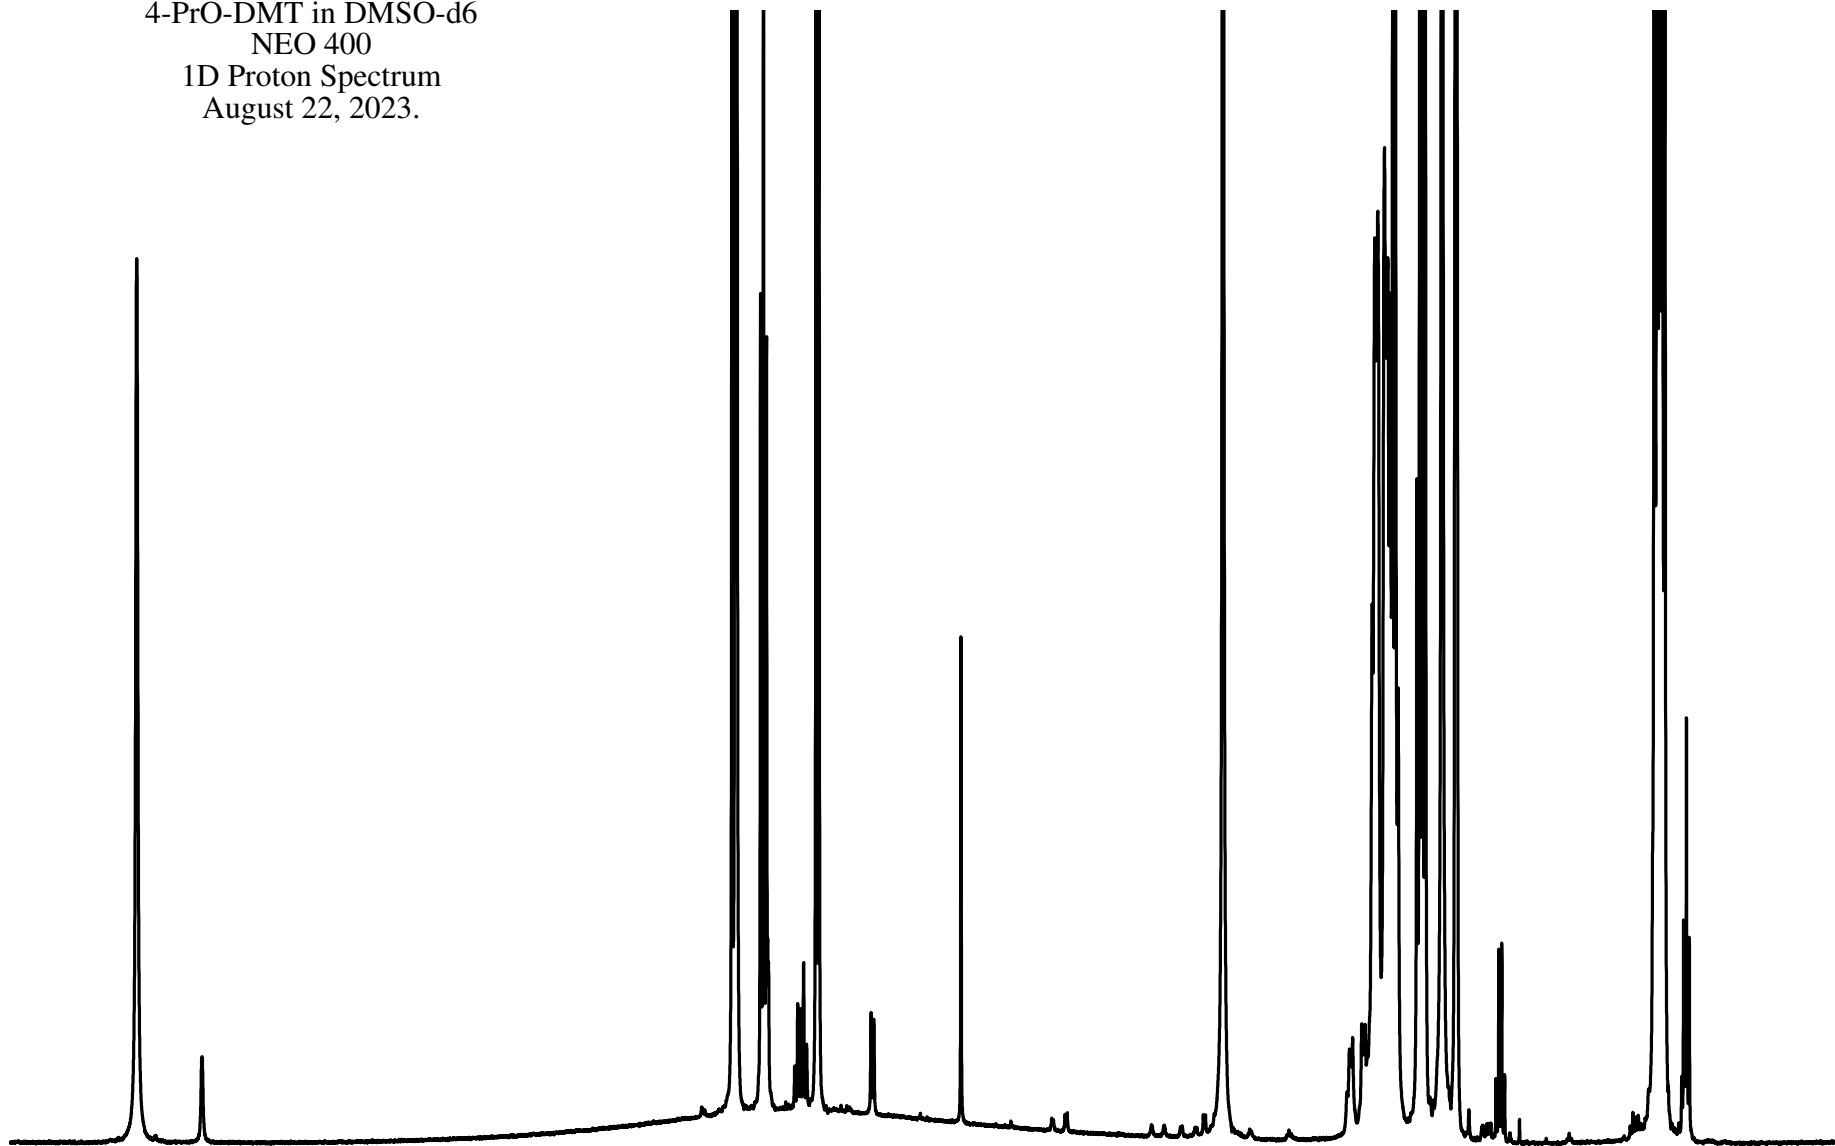


4-PrO-DMT in DMSO-d6
NEO 400
1D Proton Spectrum
August 22, 2023.

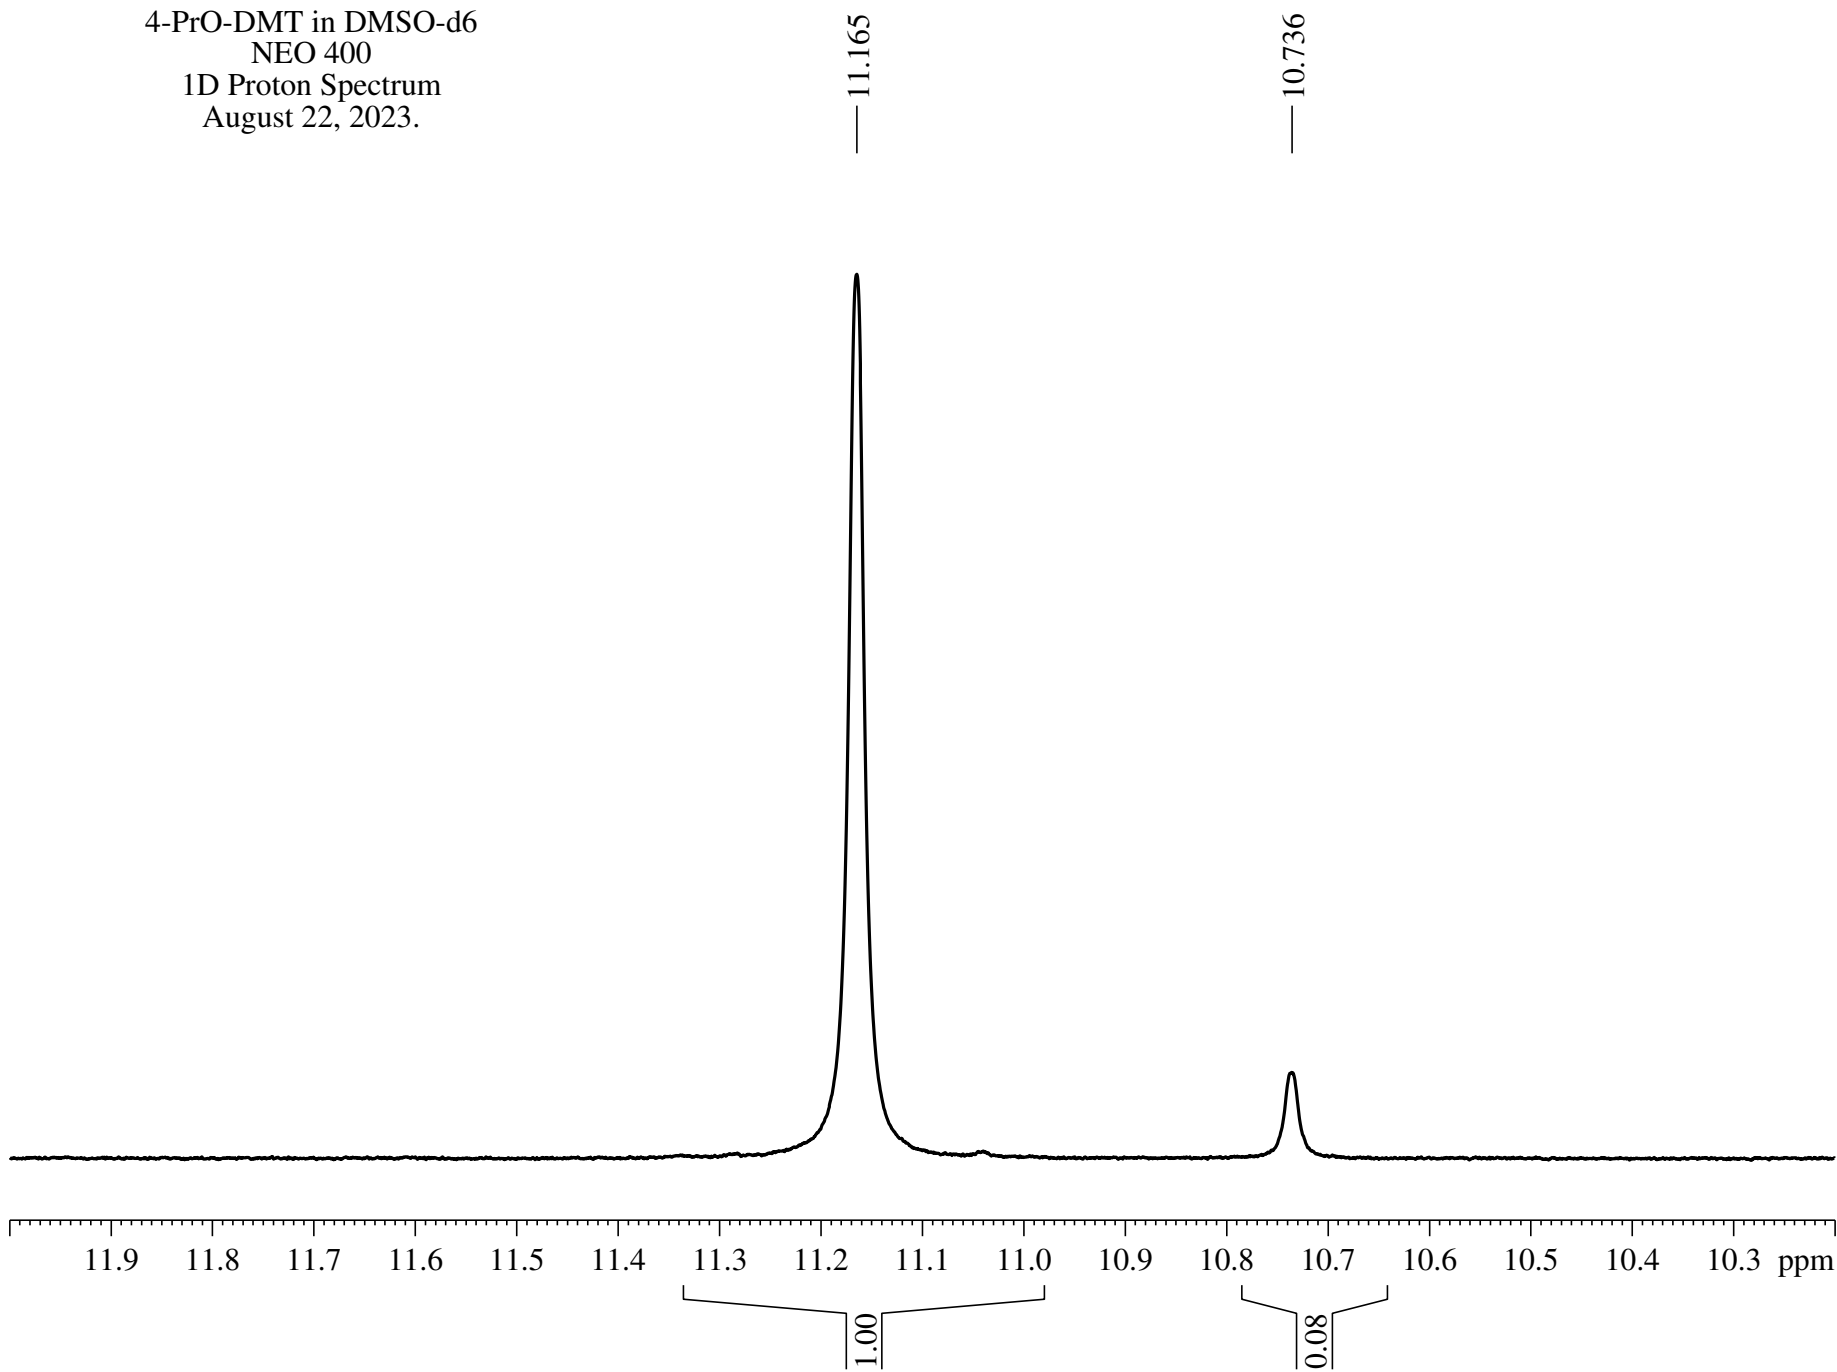

4-PrO-DMT in DMSO-d6
NEO 400
1D Proton Spectrum
August 22, 2023.

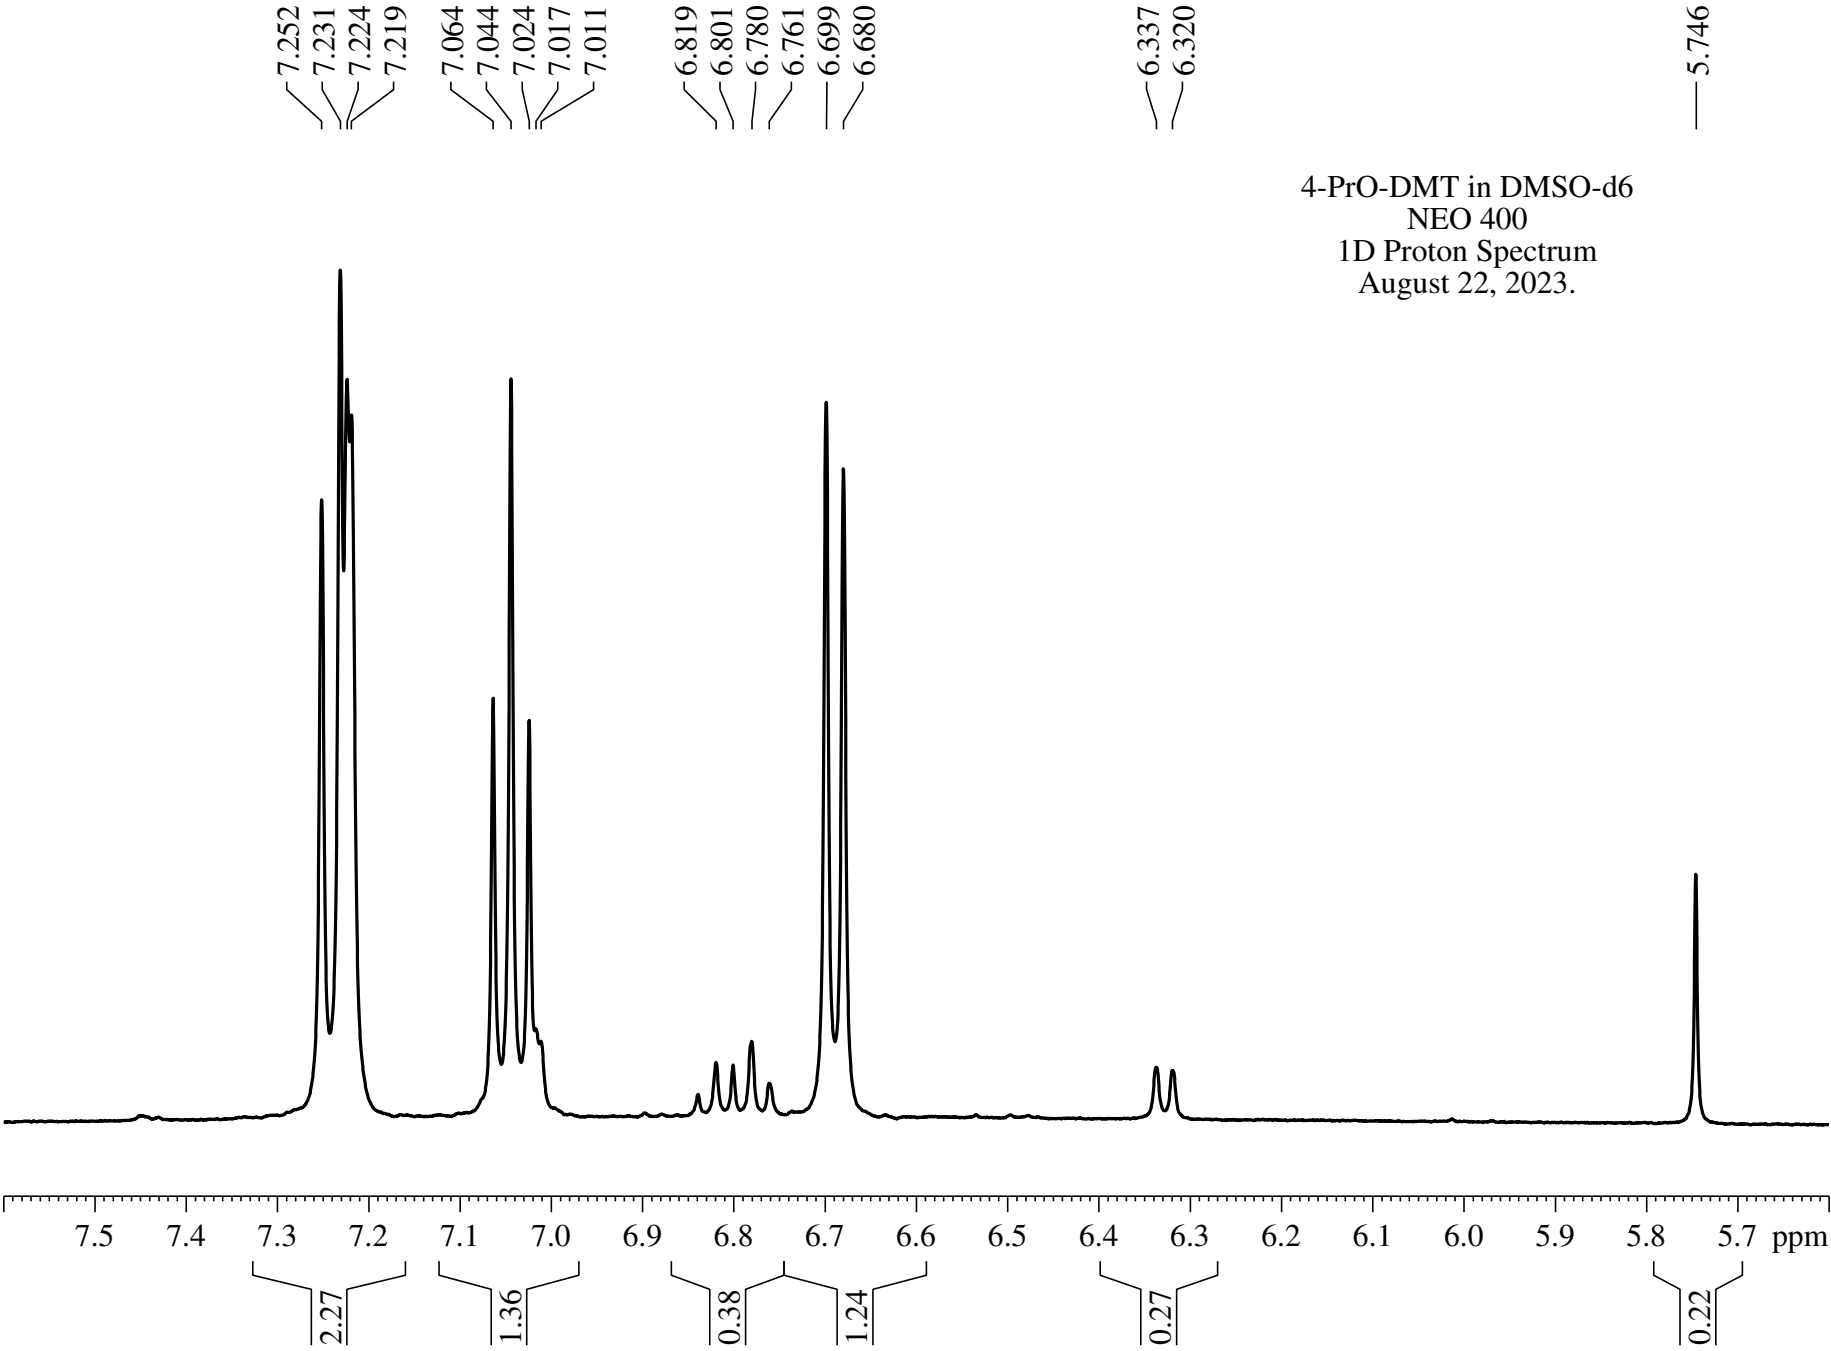

4-PrO-DMT in DMSO-d6
NEO 400
1D Proton Spectrum
August 22, 2023.

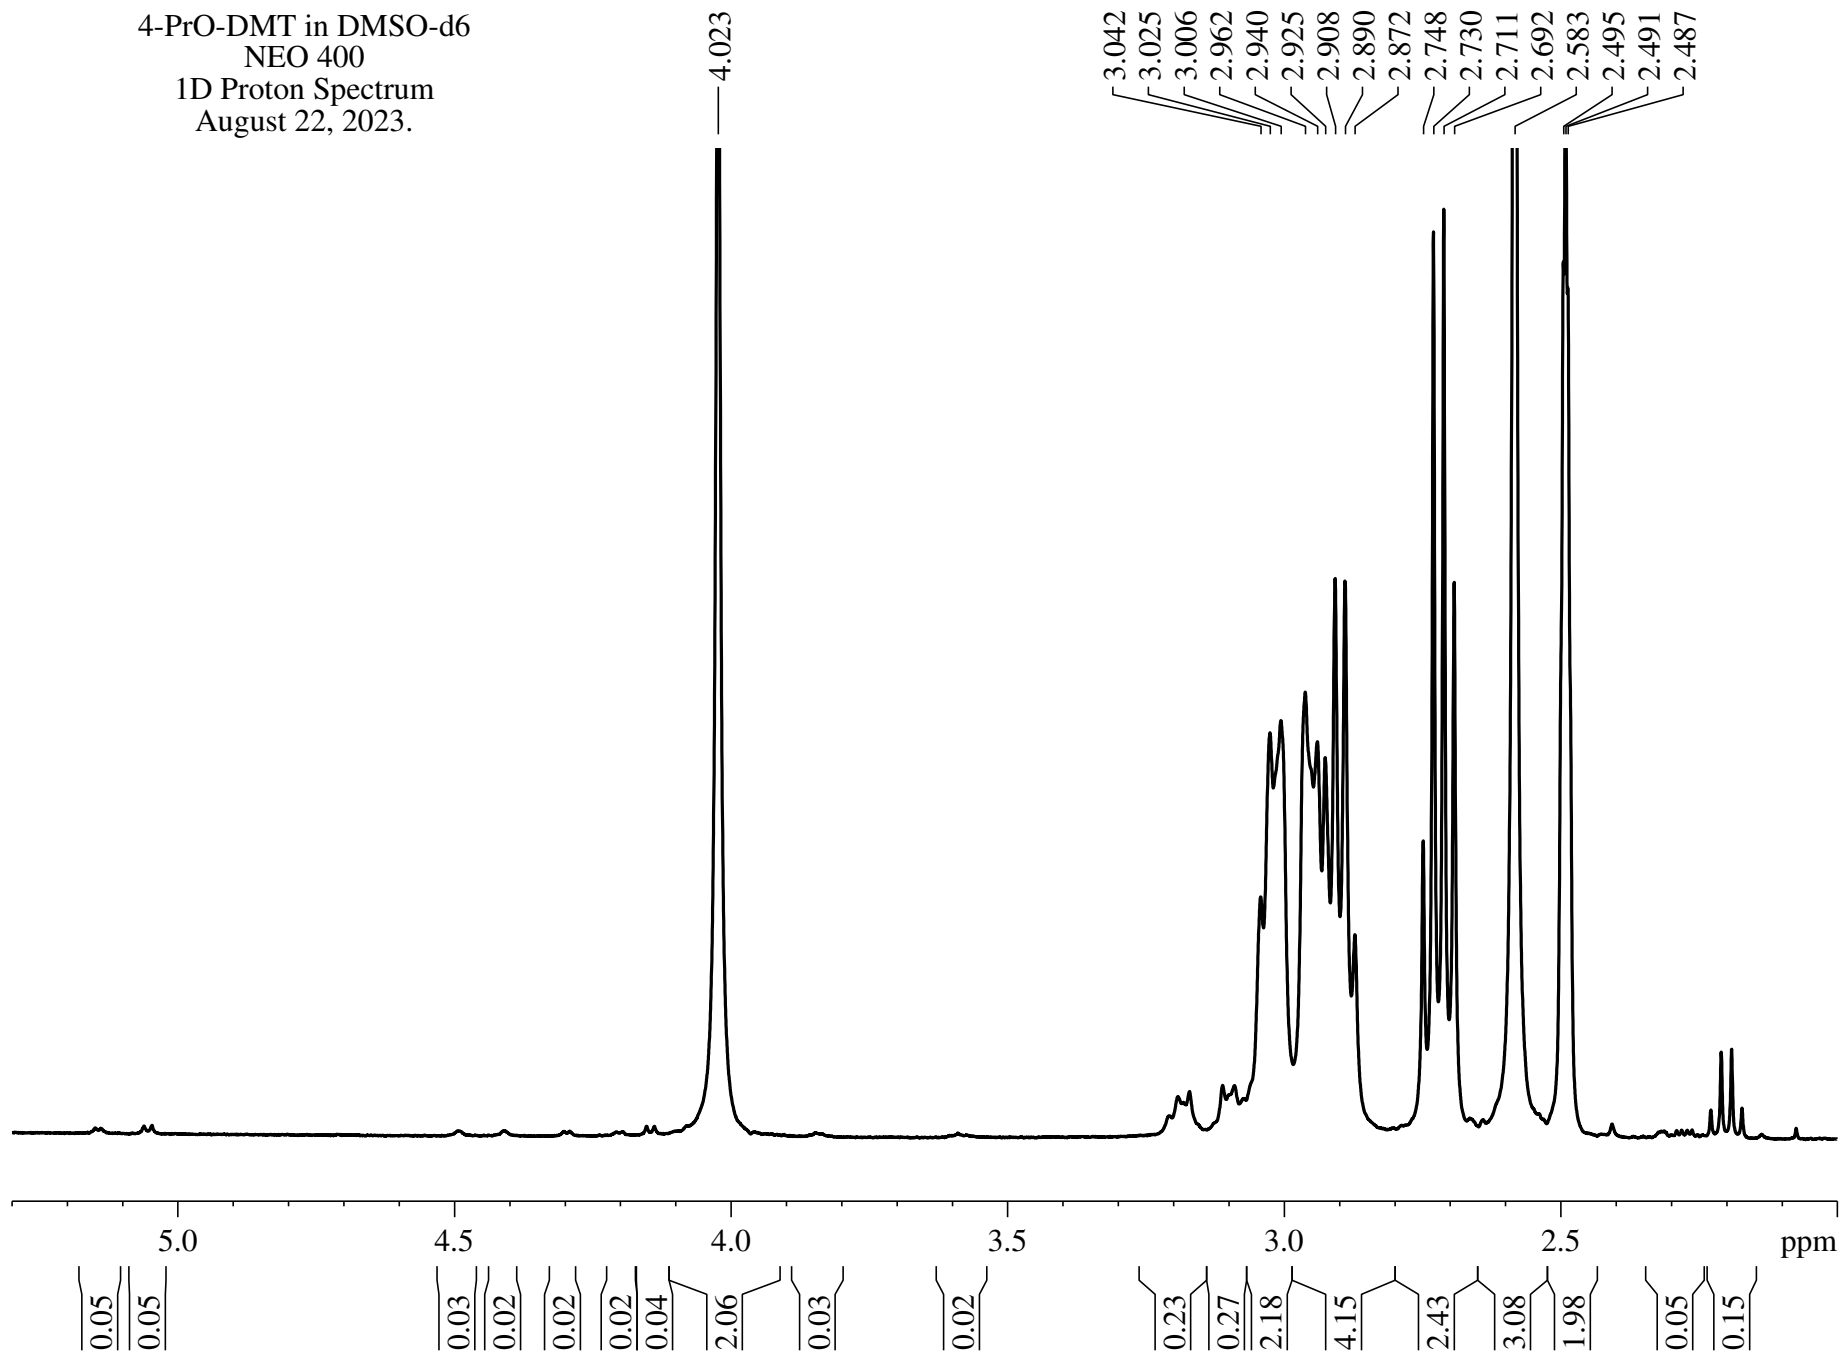

4-PrO-DMT in DMSO-d6
NEO 400
1D Proton Spectrum
August 22, 2023.

