
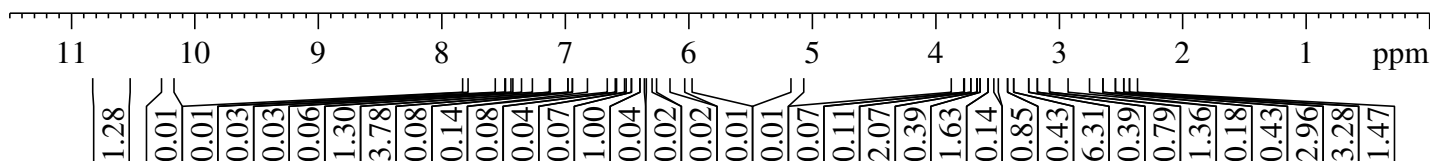


Lysergamide / LSA - in DMSO-d6
NEO 400
1D Proton Spectrum
September 13, 2023.

Current Data Parameters
NAME Syntharise091323
EXPNO 400
PROCNO 1


F2 - Acquisition Parameters
Date_ 20230913
Time 14.51 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 ()
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 296.4 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters
SI 65536
SF 400.340068 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

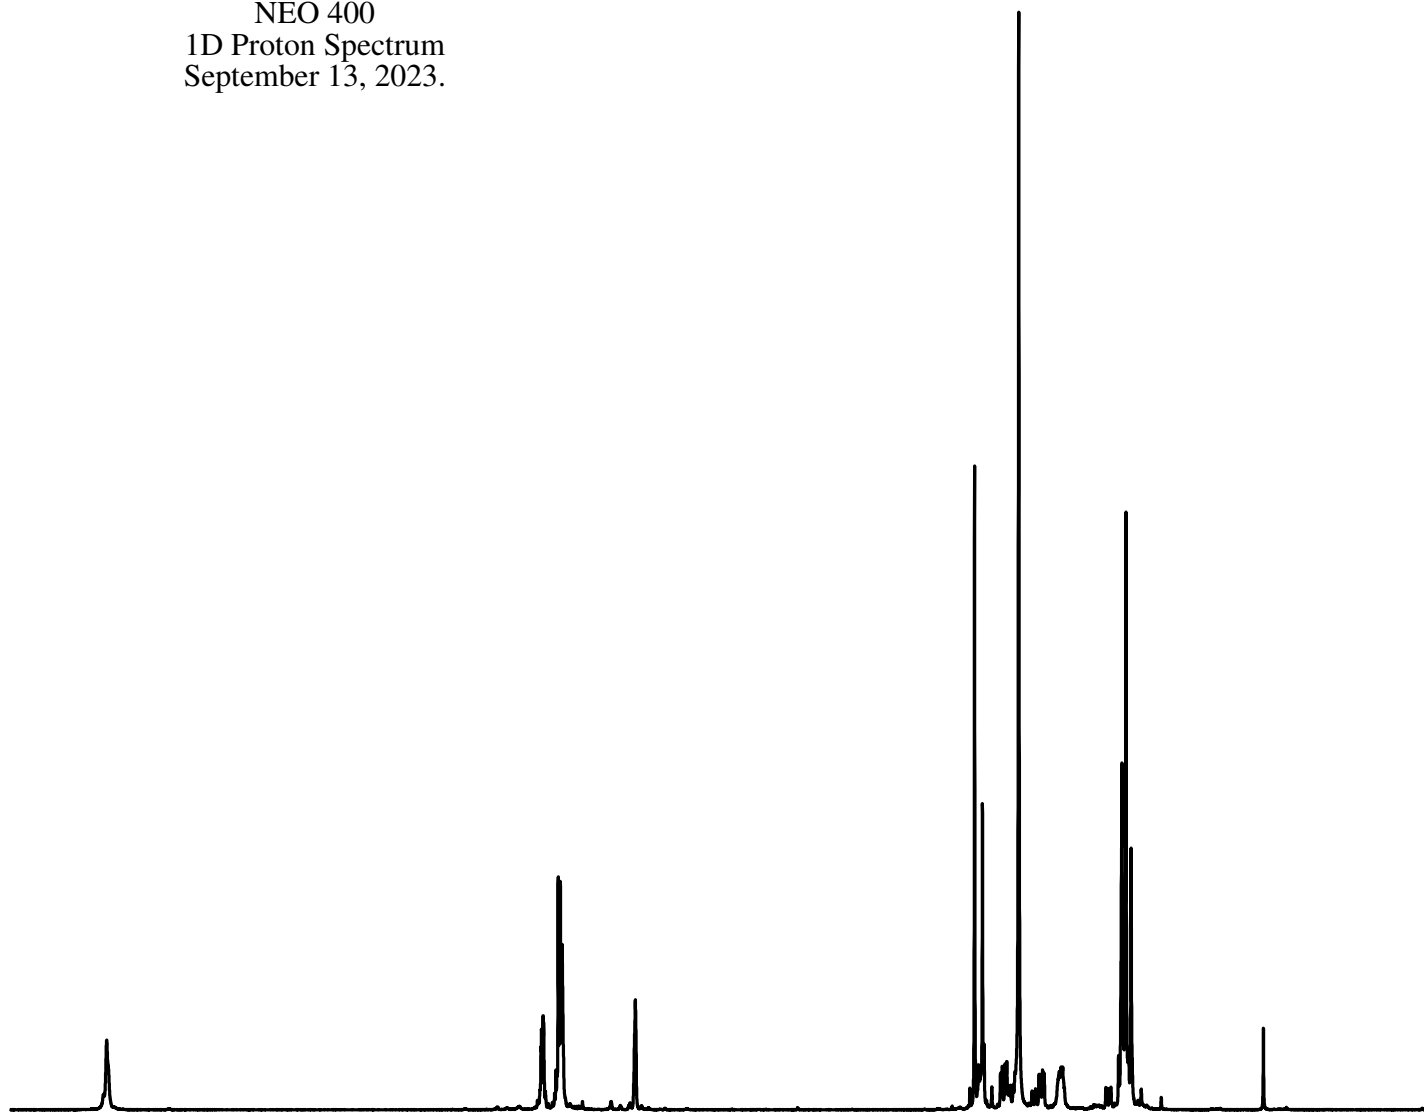

Lysergamide Fumarate in DMSO-d6
NEO 400
1D Proton Spectrum
September 13, 2023.

— 10.714

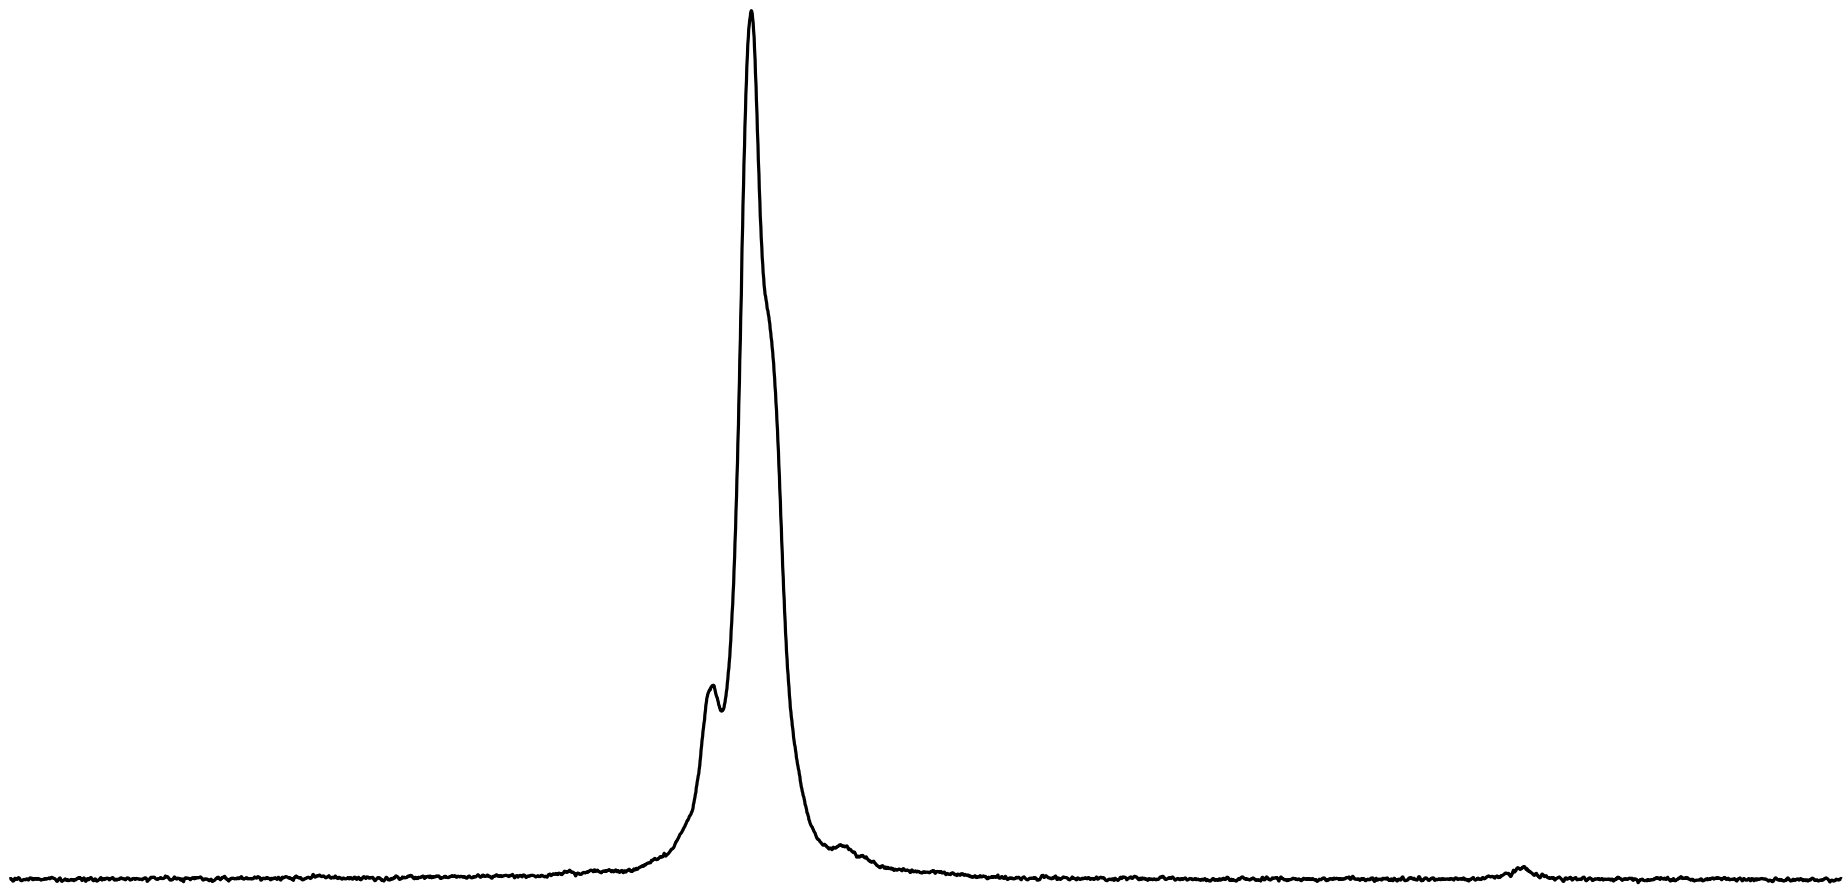

11.1 11.0 10.9 10.8 10.7 10.6 10.5 10.4 10.3 10.2 10.1 ppm



1.28

0.01


Lysergamide Fumarate in DMSO-d6
NEO 400
1D Proton Spectrum
September 13, 2023.

7.205
7.197
7.193
7.180
7.175
7.161
7.086
7.076
7.067
7.057
7.049
7.040
7.026

6.433

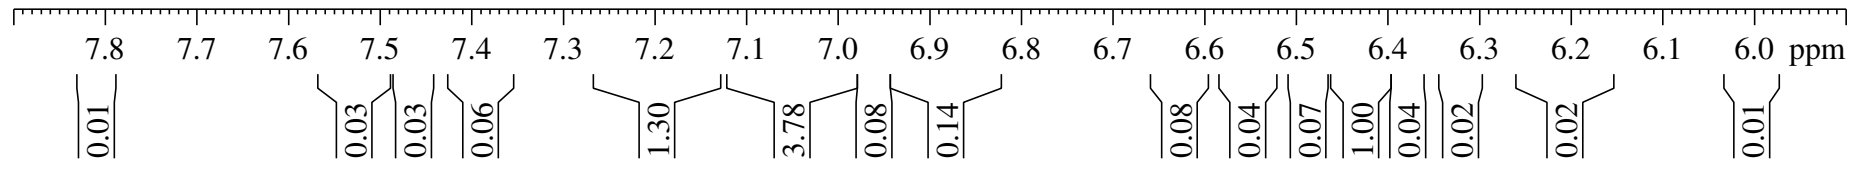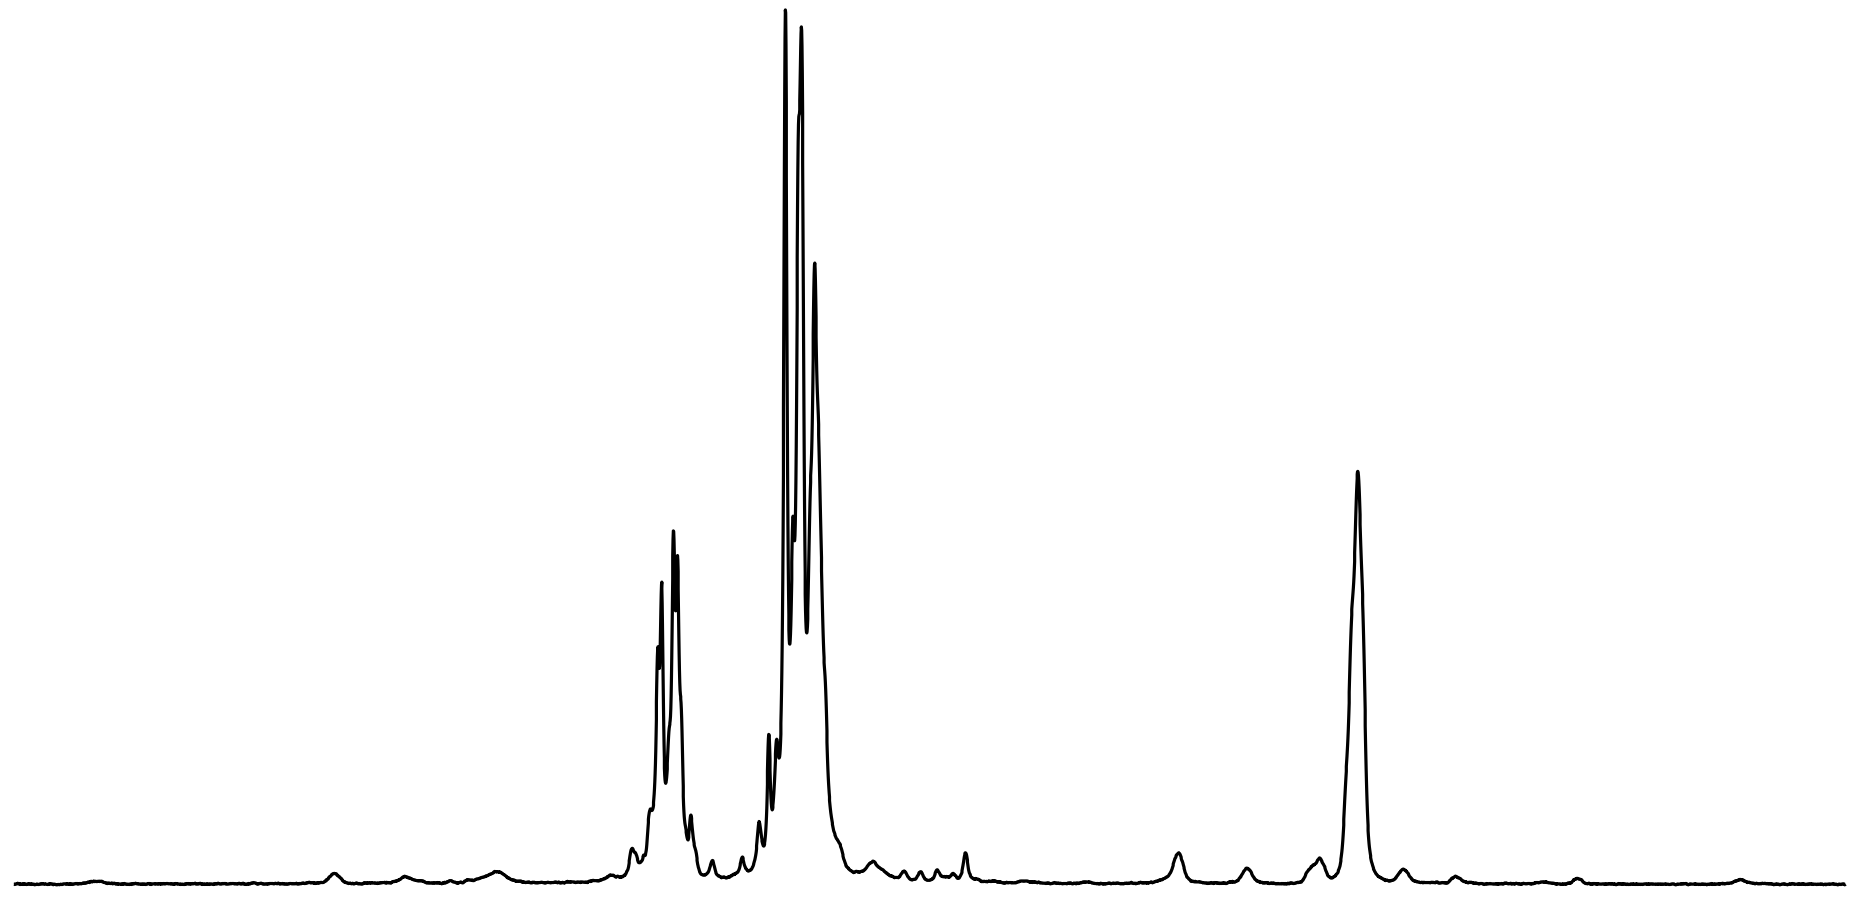

Lysergamide Fumarate in DMSO-d6
NEO 400
1D Proton Spectrum
September 13, 2023.

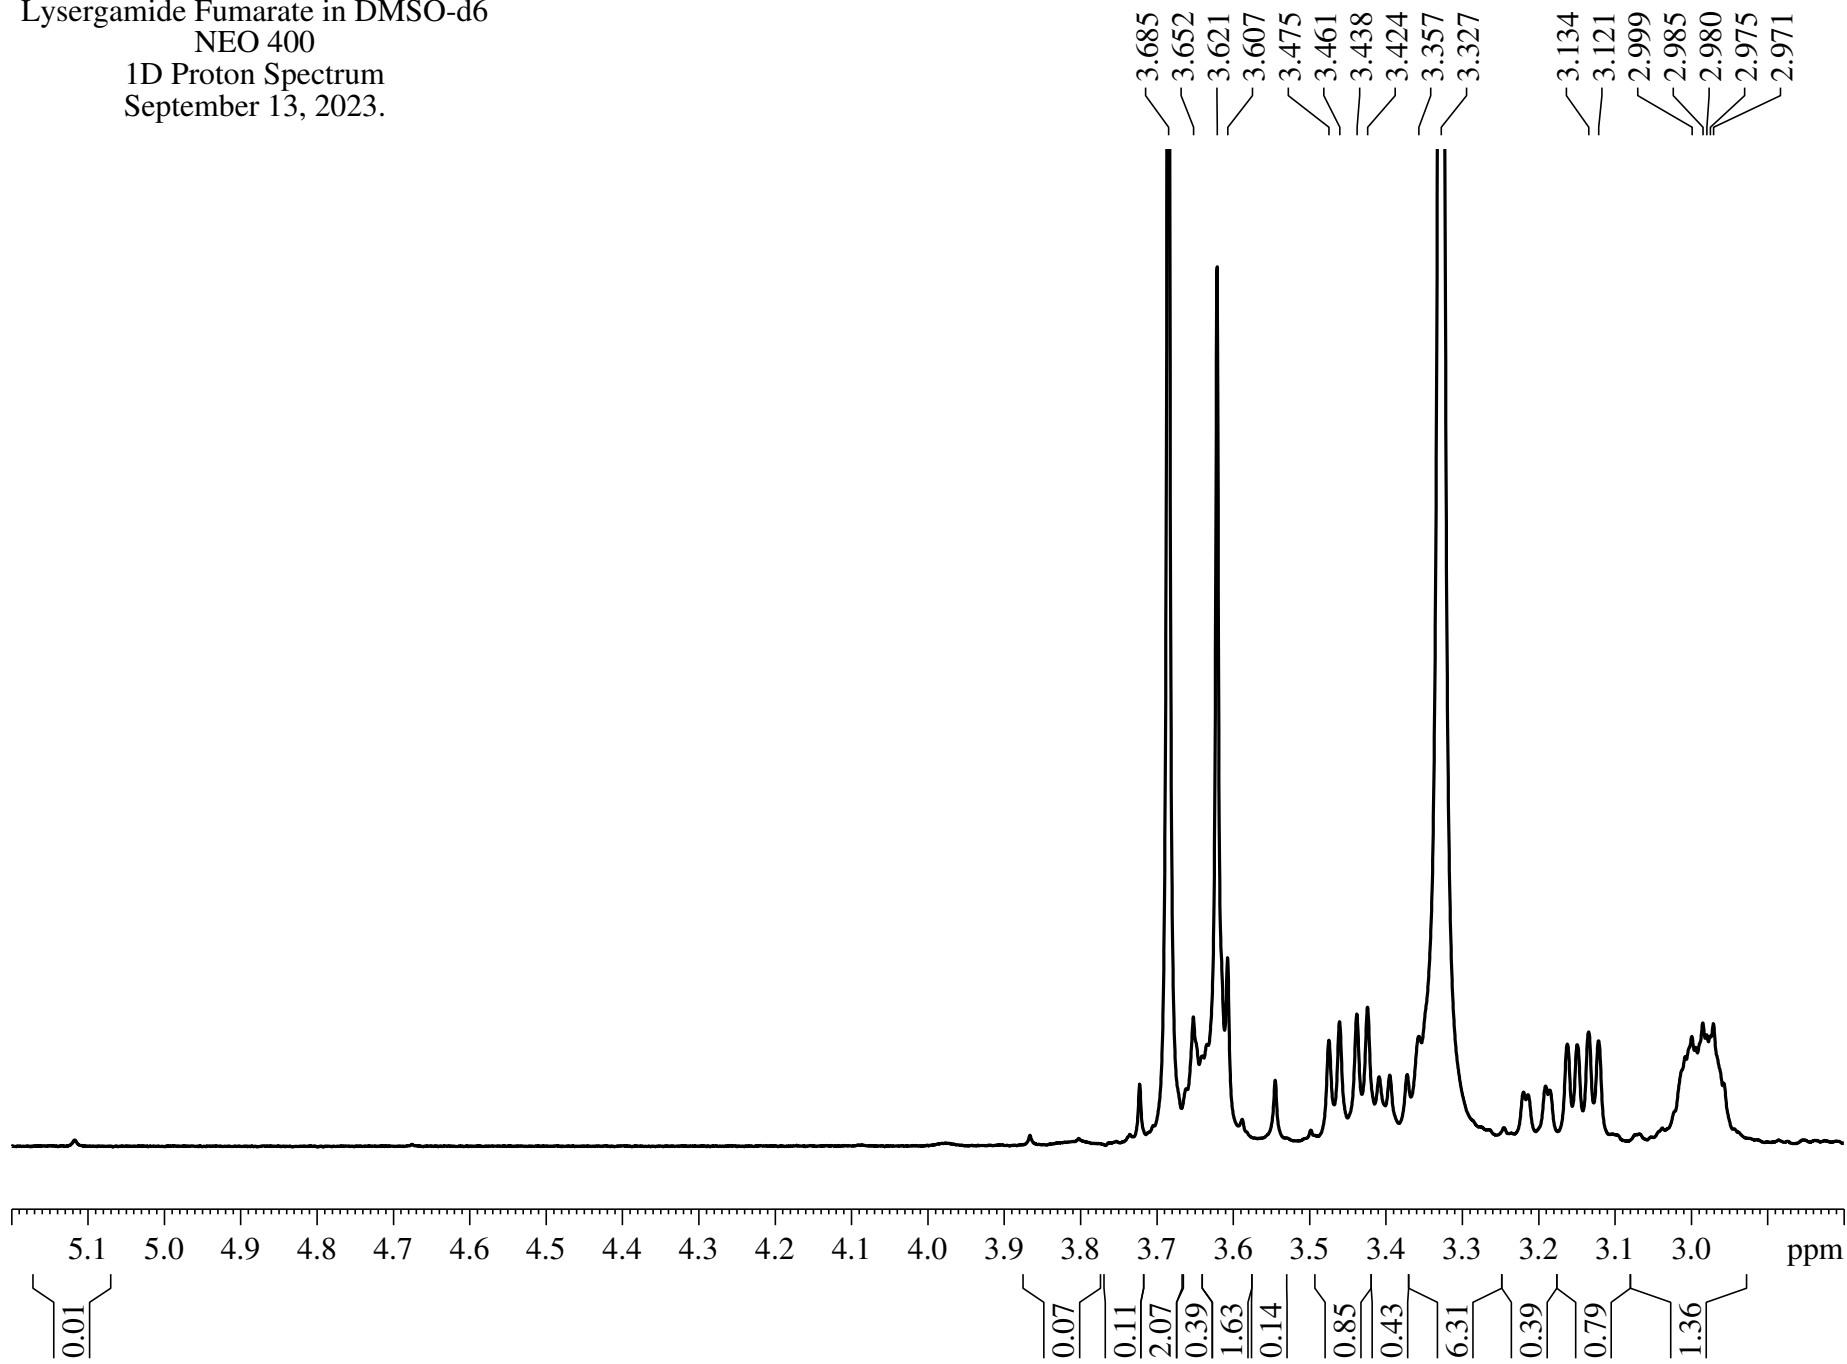

Lysergamide Fumarate in DMSO-d6
NEO 400
1D Proton Spectrum
September 13, 2023.

— 1.345

