


5MeO-sBT in DMSO-d6
NEO 400
1D Proton Spectrum
April 23, 2024.

Current Data Parameters
NAME Syntharise042324
EXPNO 410
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240423
Time 12.56 h
INSTRUM Avance Neo 400
PROBHD Z104450_0313 (zg30)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 298.2 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W



F2 - Processing parameters
SI 65536
SF 400.340066 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

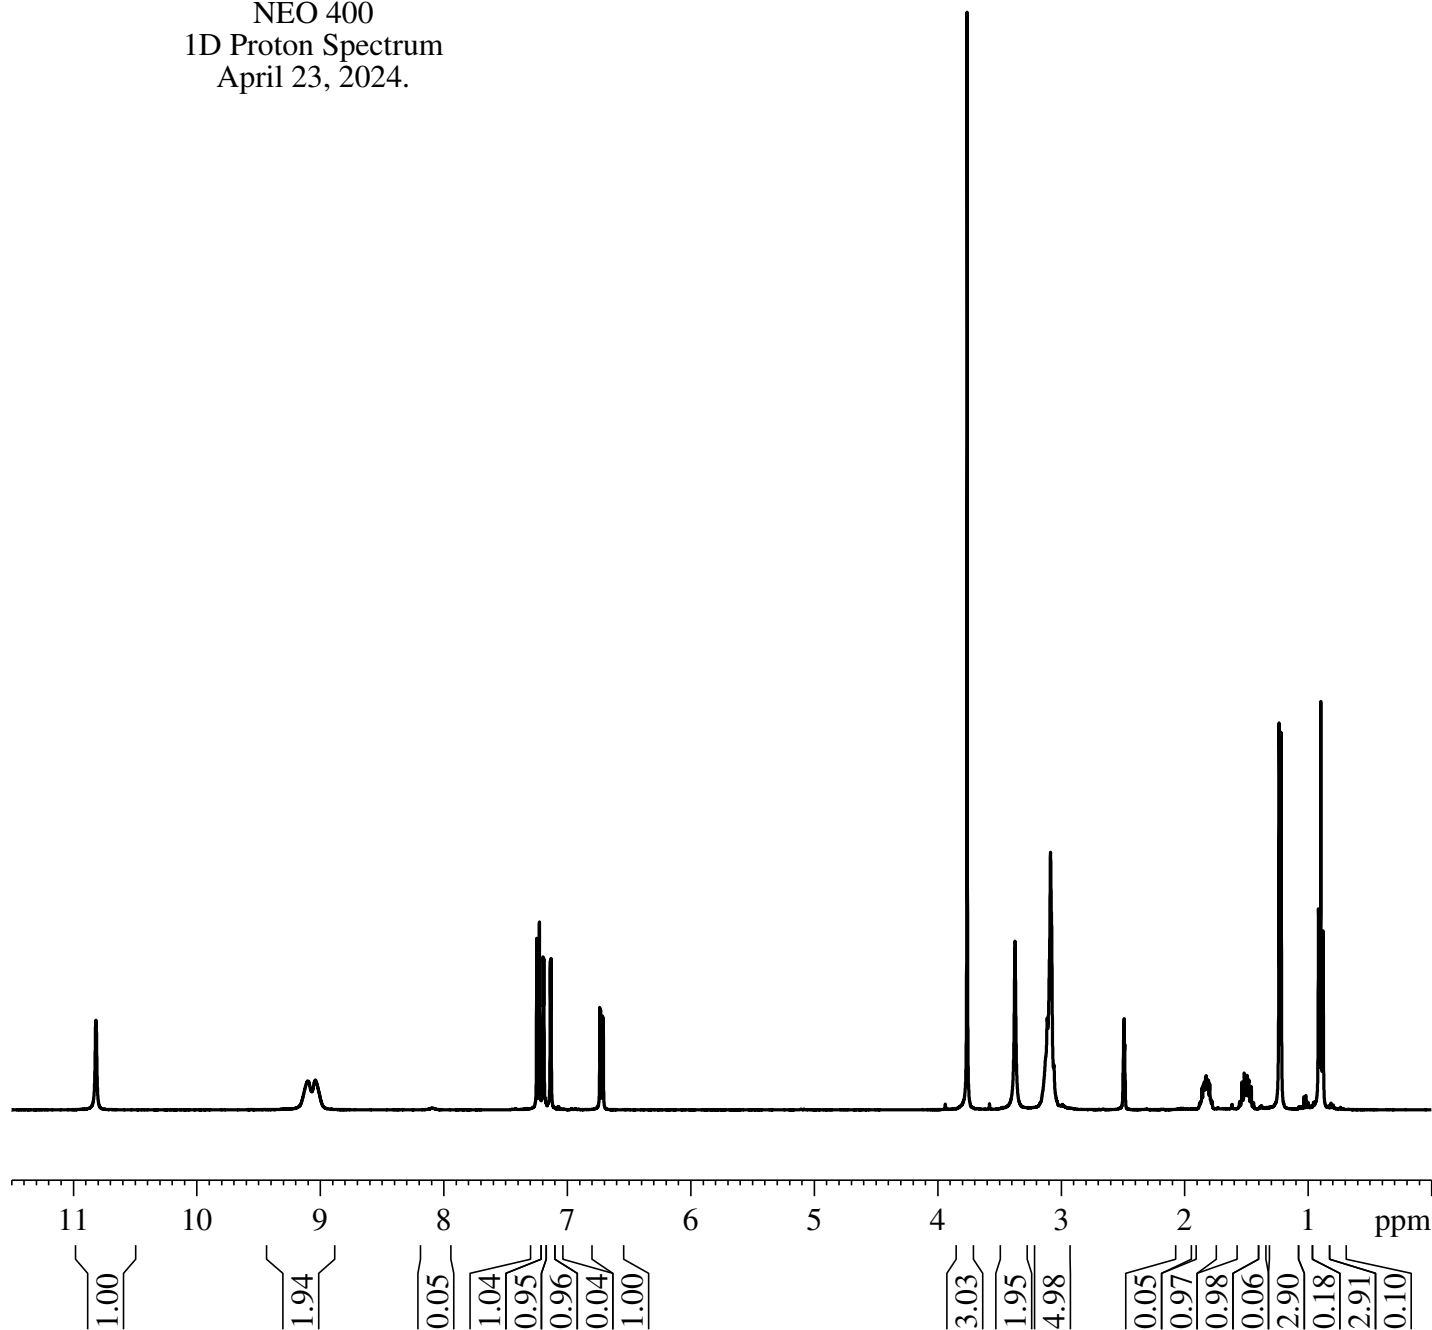

5MeO-sBT in DMSO-d6
NEO 400
1D Proton Spectrum
April 23, 2024.

— 10.818



— 9.101
— 9.040

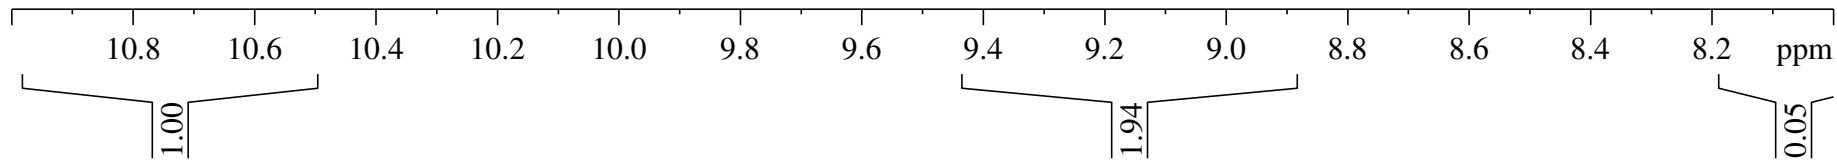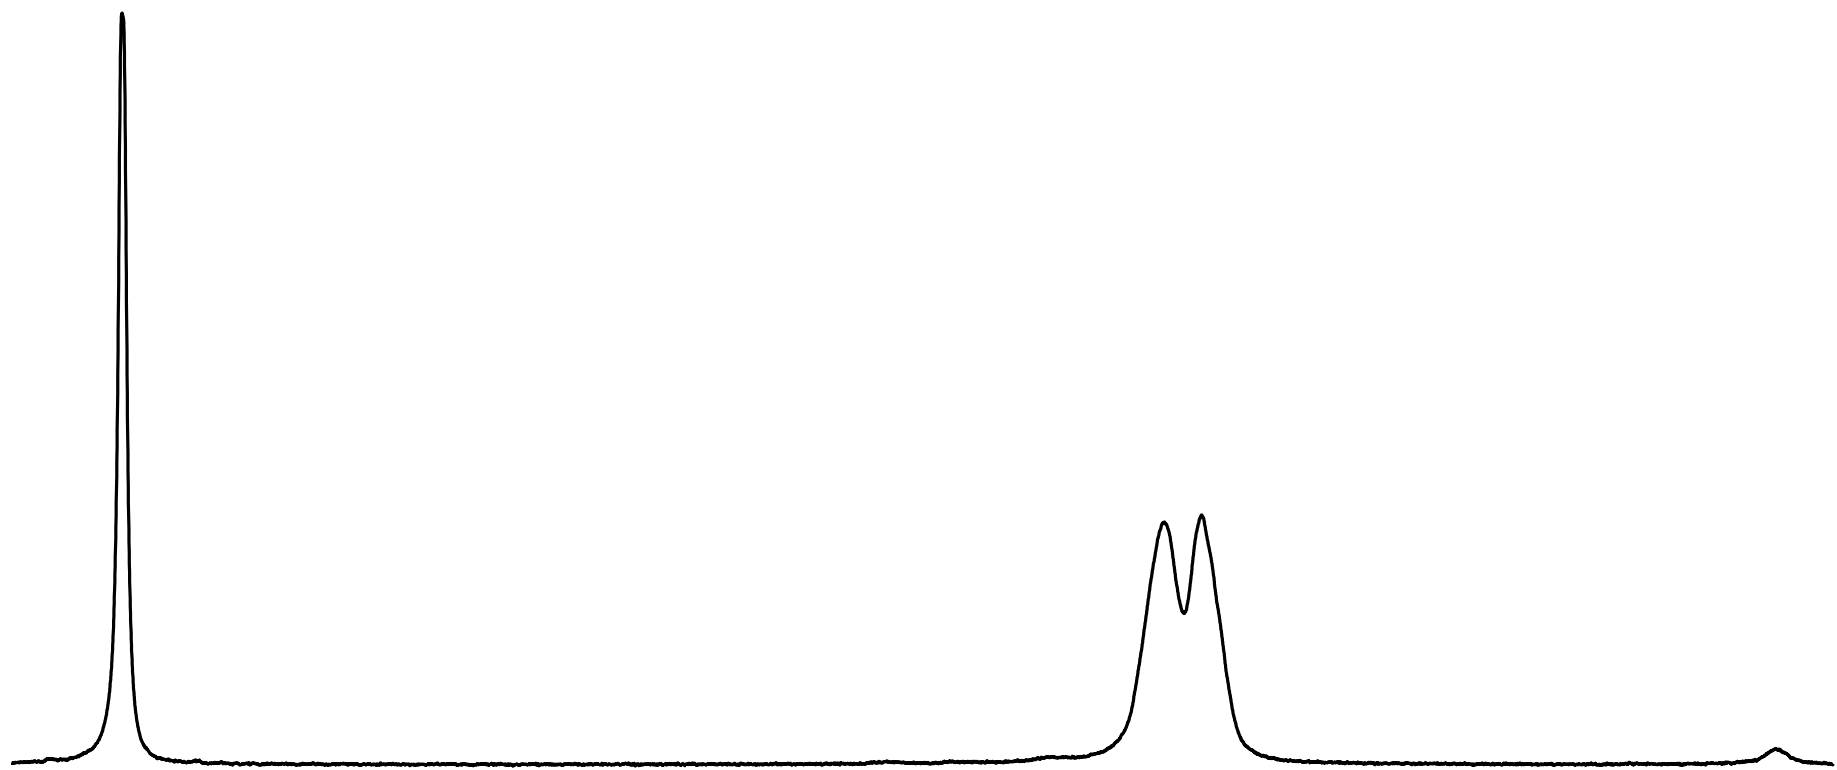


7.248
7.226
7.196
7.190
7.137
7.132

5MeO-sBT in DMSO-d6
NEO 400
1D Proton Spectrum
April 23, 2024.

6.737
6.731
6.715
6.709

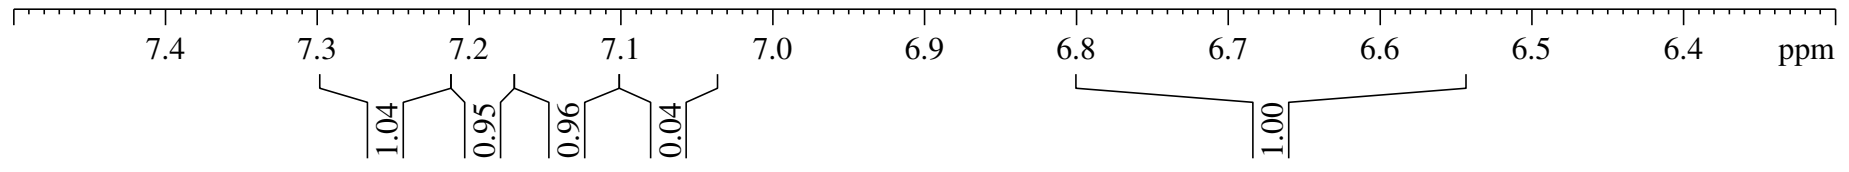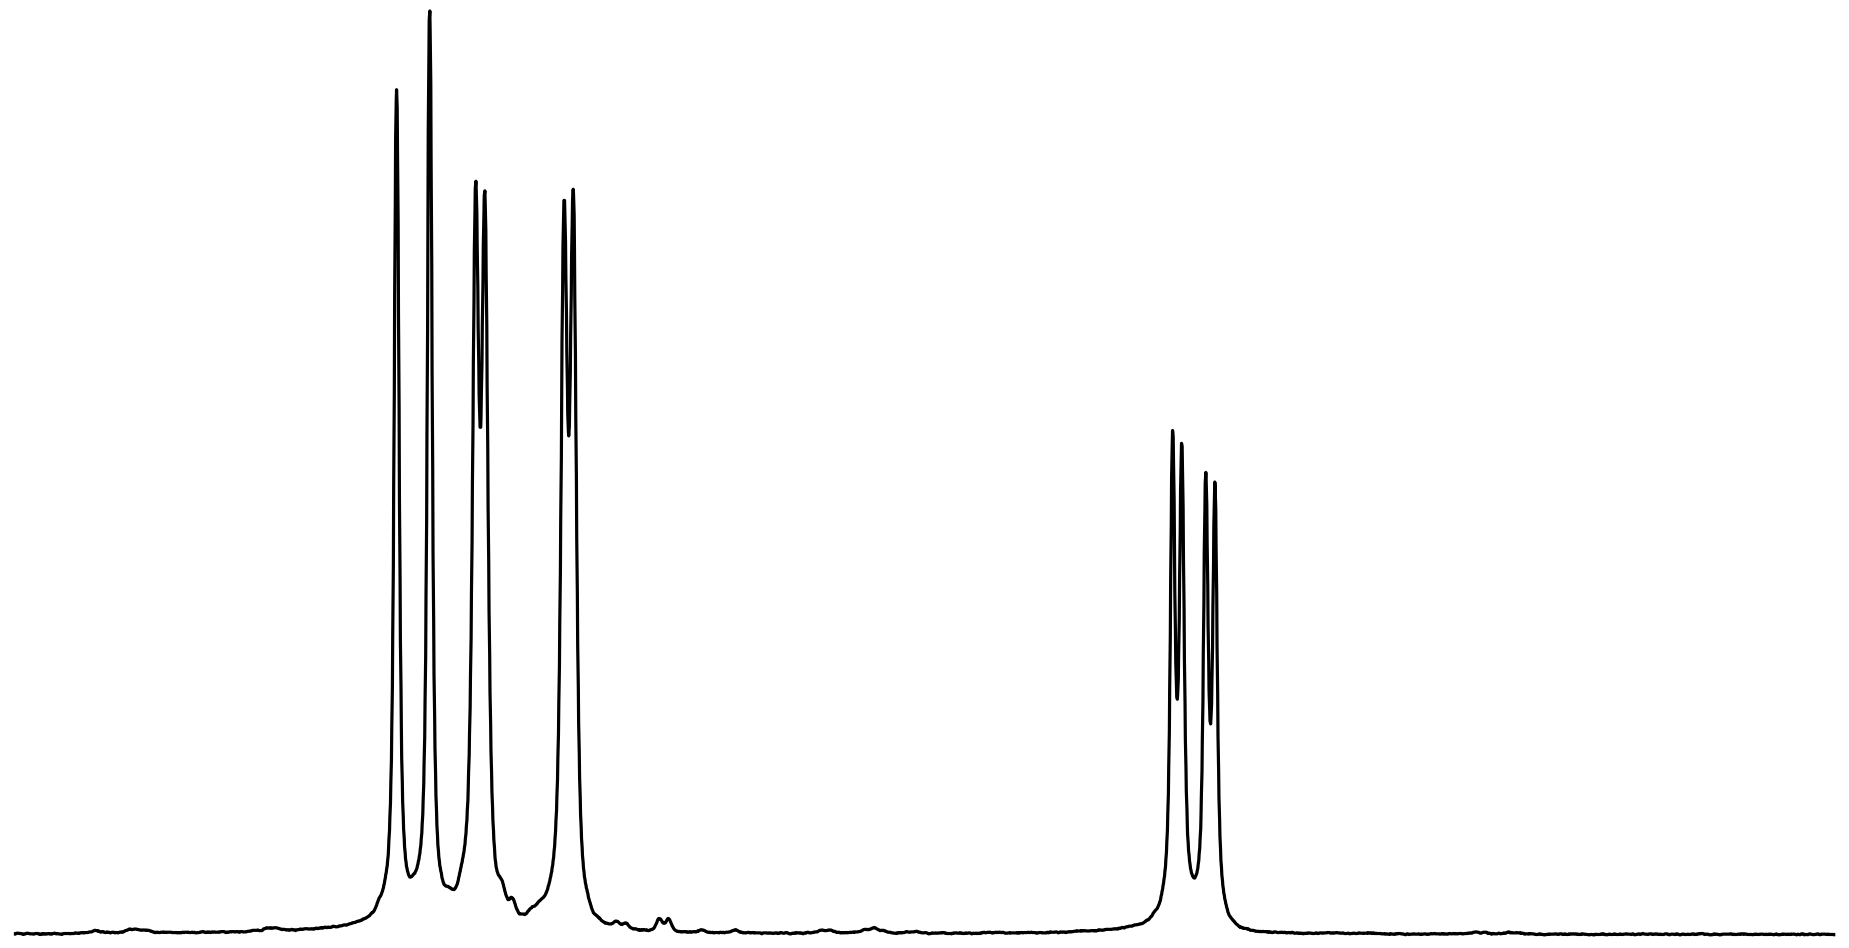

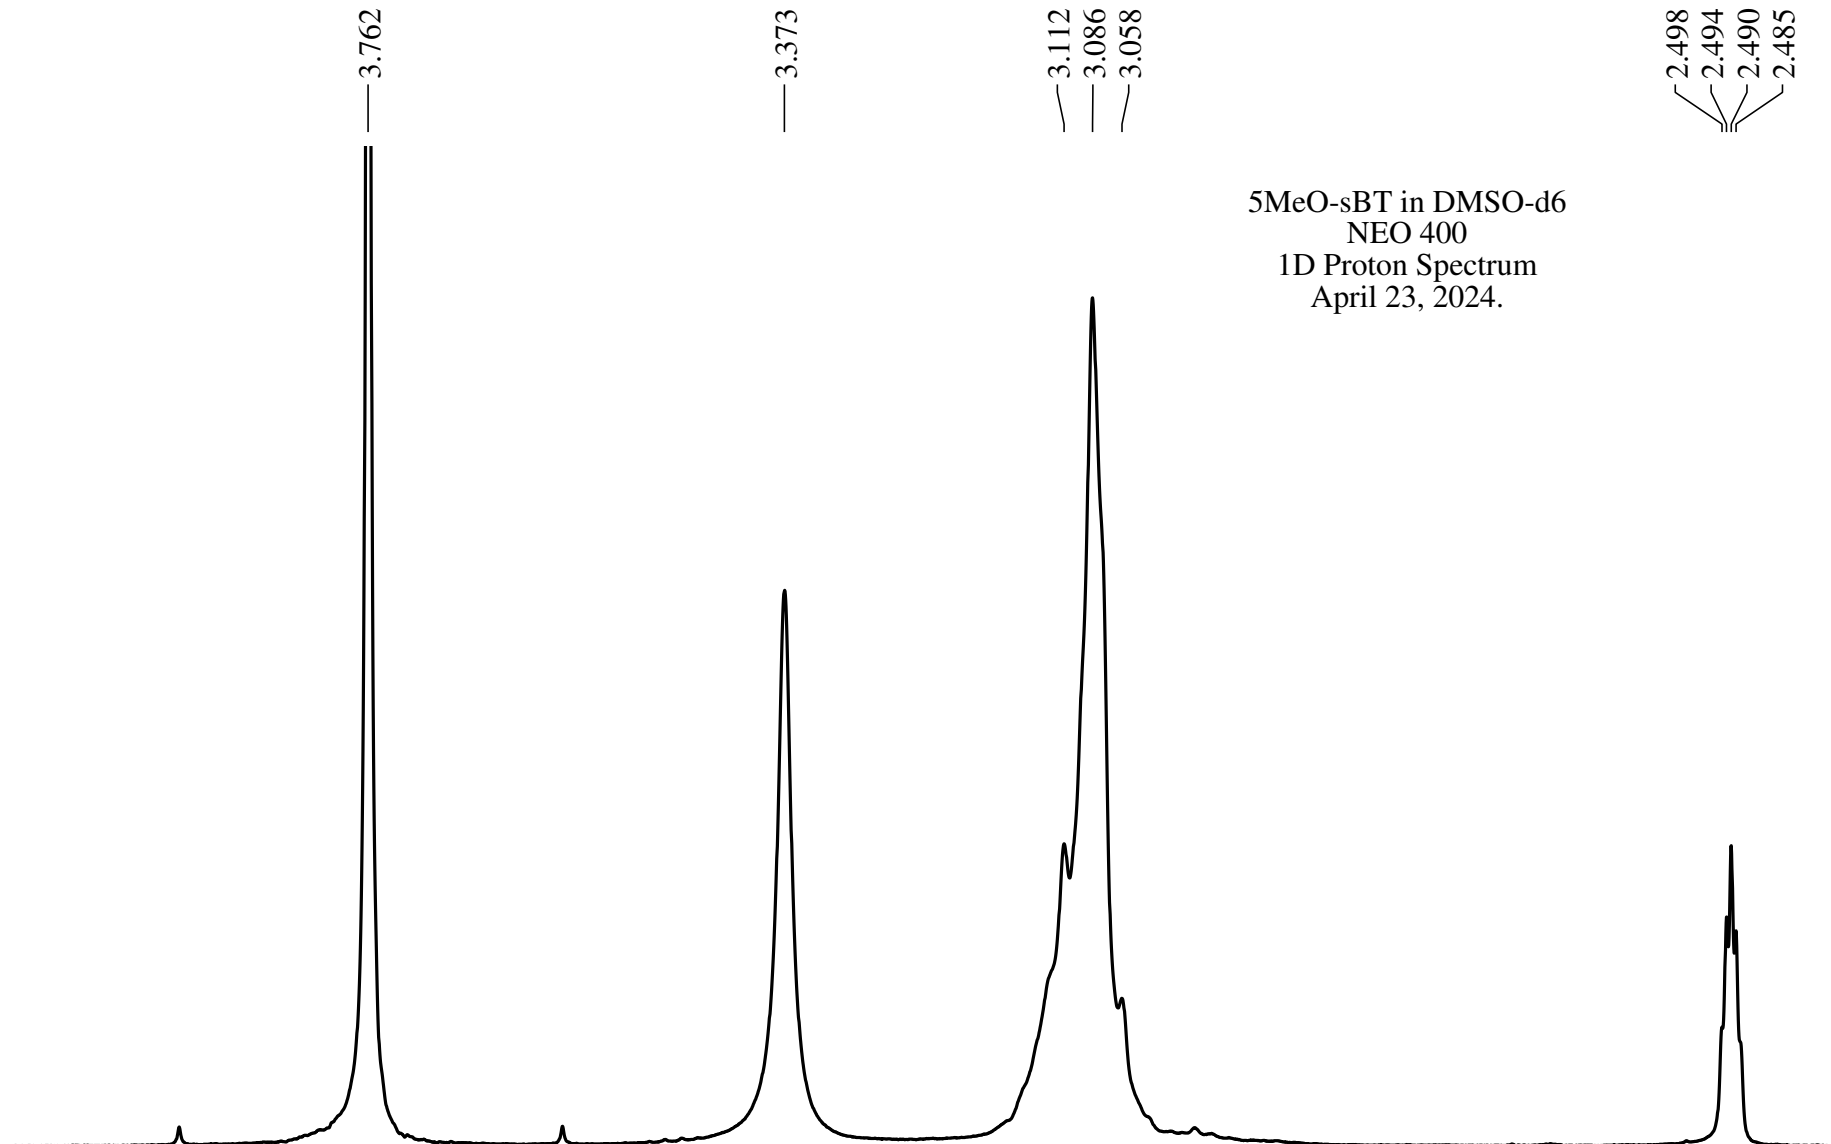

5MeO-sBT in DMSO-d6
NEO 400
1D Proton Spectrum
April 23, 2024.

3.762

3.373

3.112

3.086

3.058

2.498

2.494

2.490

2.485

4.0 3.9 3.8 3.7 3.6 3.5 3.4 3.3 3.2 3.1 3.0 2.9 2.8 2.7 2.6 2.5 ppm

3.03

1.95

4.98


1.859
1.849
1.840
1.830
1.826
1.816
1.807
1.797

1.535
1.517
1.513
1.501
1.494
1.483
1.479
1.460

1.235
1.218

0.915
0.897
0.878

5MeO-sBT in DMSO-d6
NEO 400
1D Proton Spectrum
April 23, 2024.

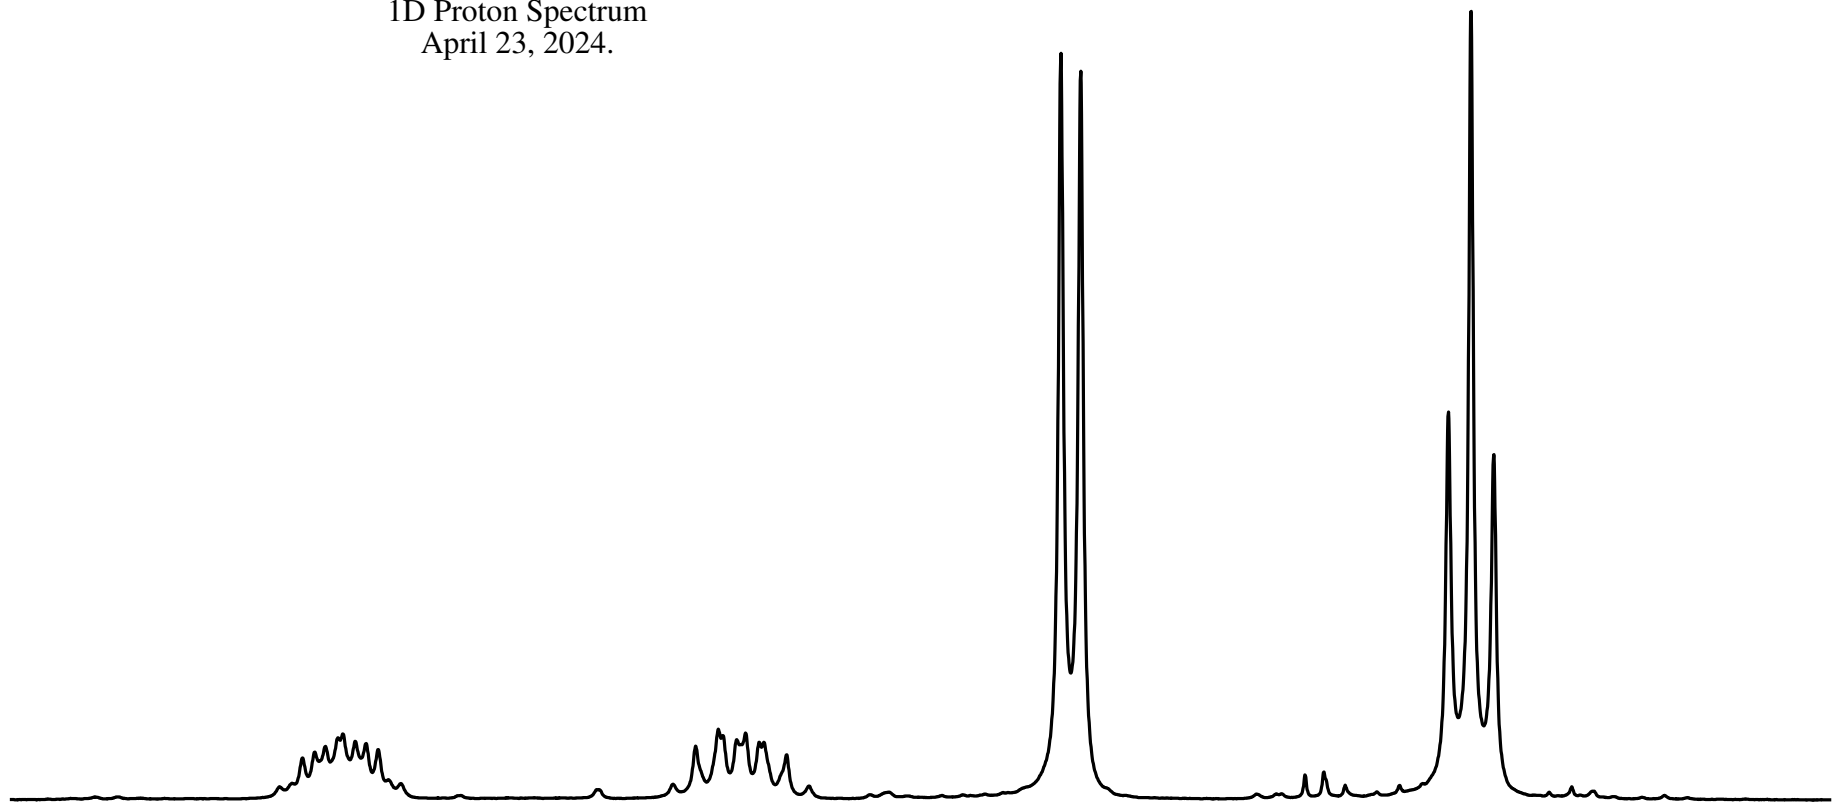

2.0 1.9 1.8 1.7 1.6 1.5 1.4 1.3 1.2 1.1 1.0 0.9 0.8 0.7 ppm

0.05 0.97 0.98 0.06 2.90 0.18 2.91 0.10