


Chloretazopyzine DMSO-d6
NEO 400
1D Proton Spectrum
February 5, 2025.

Current Data Parameters
NAME Syntharise020525
EXPNO 440
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250205
Time 15.08 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 (PI HR-400-S
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 295.9 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W


F2 - Processing parameters
SI 65536
SF 400.3400069 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

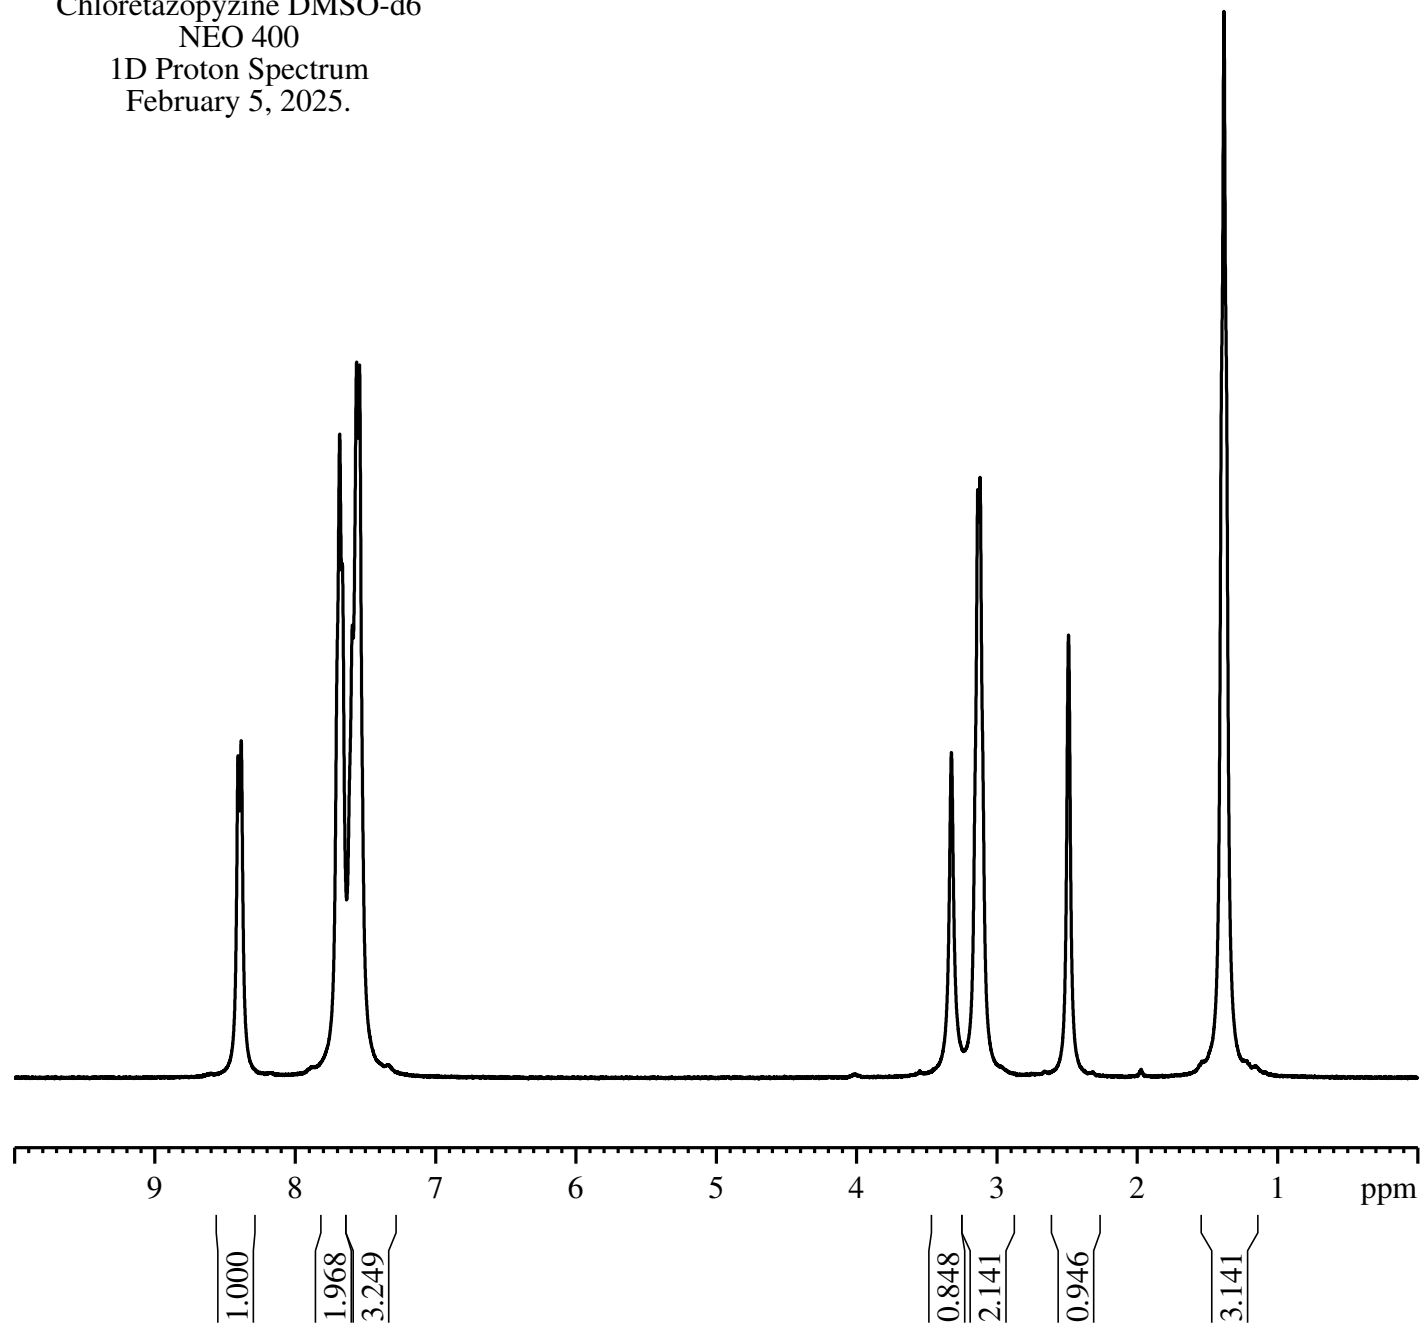

8.406
8.384

Chloretazopyzine DMSO-d6
NEO 400
1D Proton Spectrum
February 5, 2025.

7.682
7.664
7.592
7.562
7.541

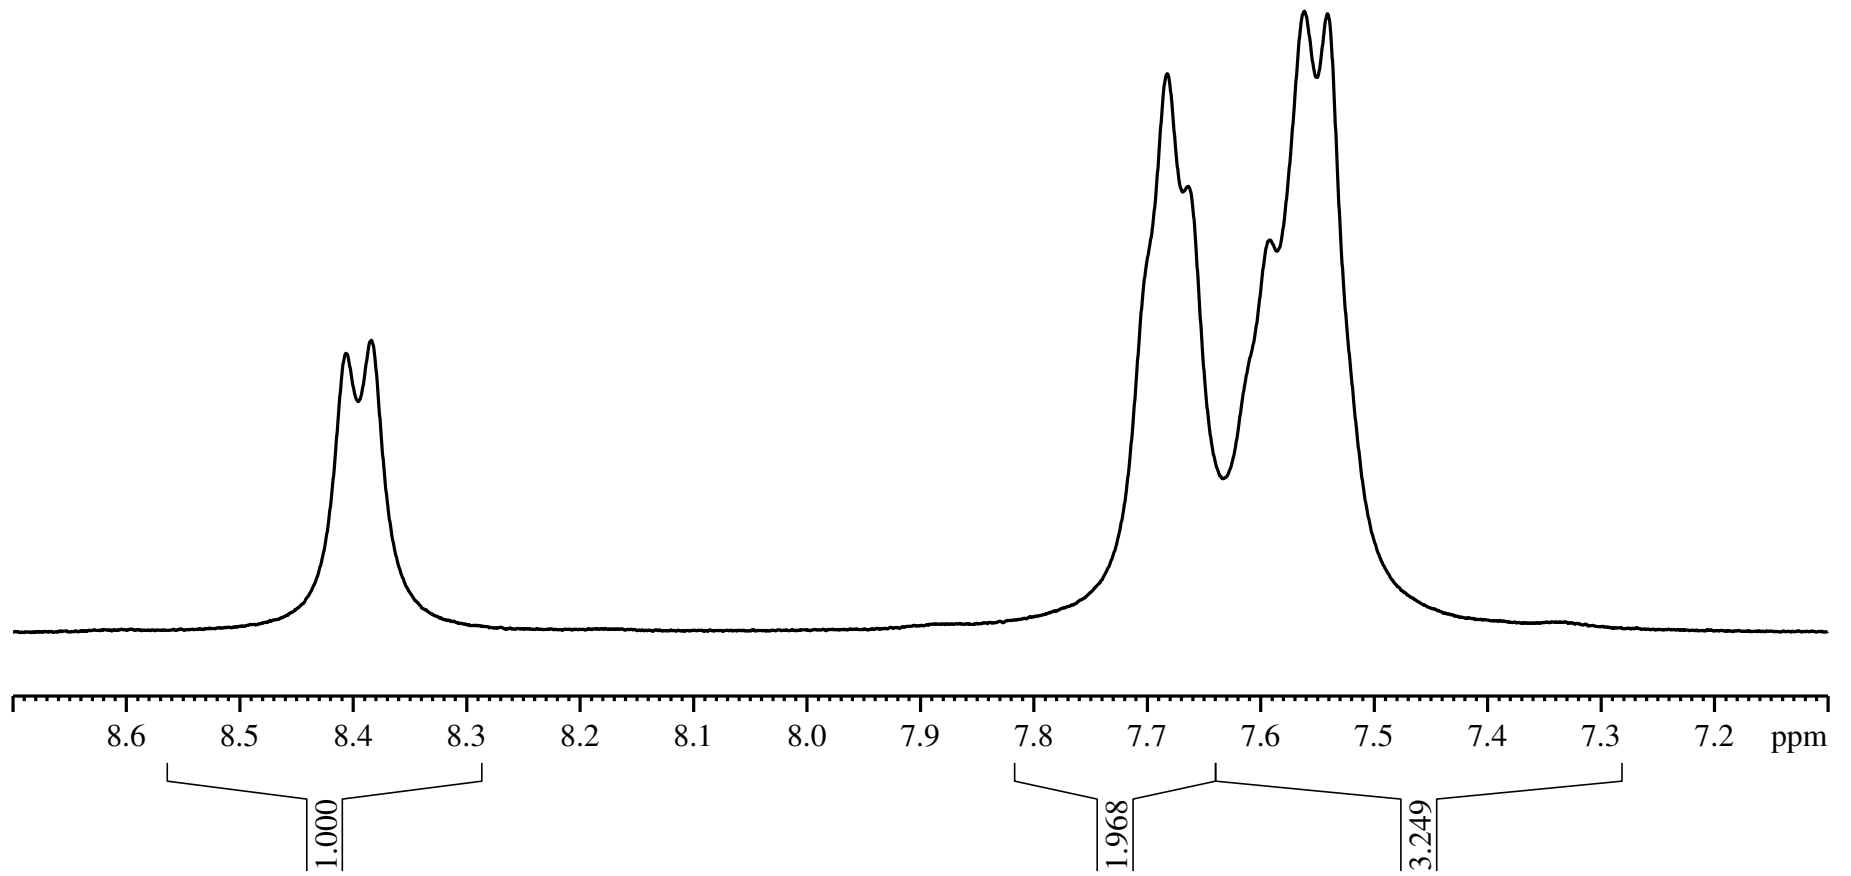

Chloretazopyzine DMSO-d6
NEO 400
1D Proton Spectrum
February 5, 2025.

