


LTA in DMSO-d6
NEO 400
1D Proton Spectrum
February 25, 2025.

Current Data Parameters
NAME Syntharise022525
EXPNO 470
PROCNO 1


F2 - Acquisition Parameters
Date_ 20250225
Time 13.56 h
INSTRUM Avance Neo 400
PROBHD Z104450_0313 (PA BBO 400)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 297.3 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters
SI 65536
SF 400.3400060 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

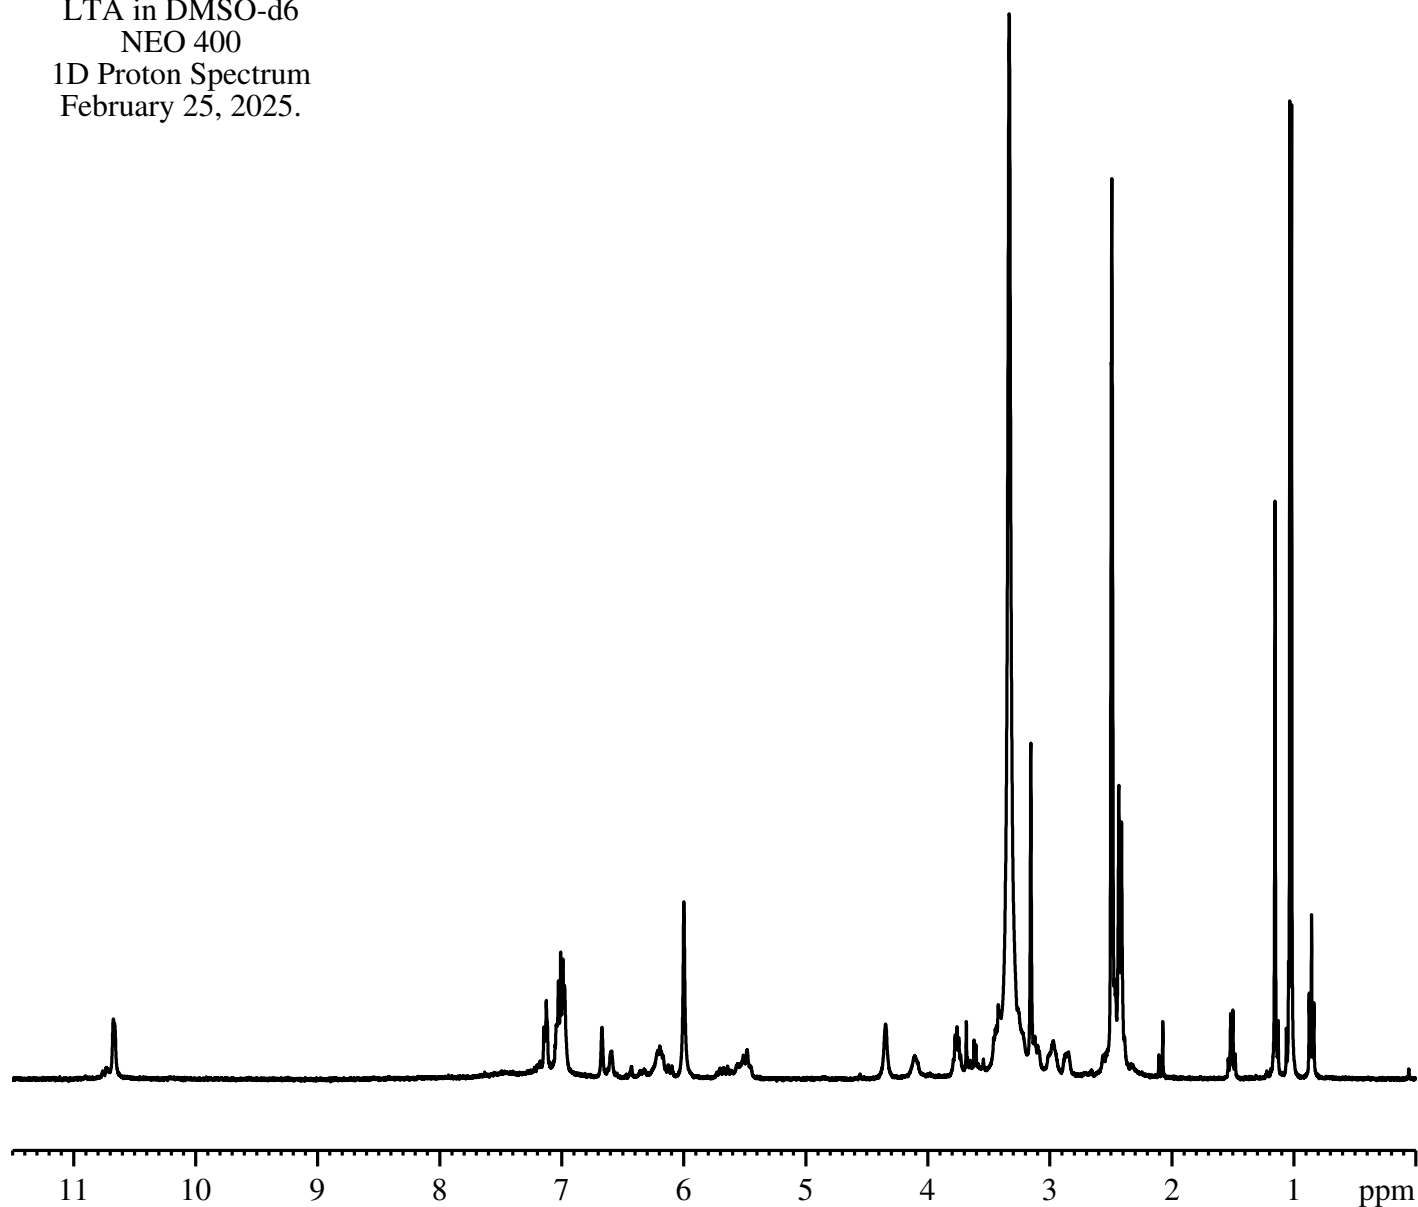

LTA in DMSO-d6
NEO 400
1D Proton Spectrum
February 25, 2025.


10.673
10.663

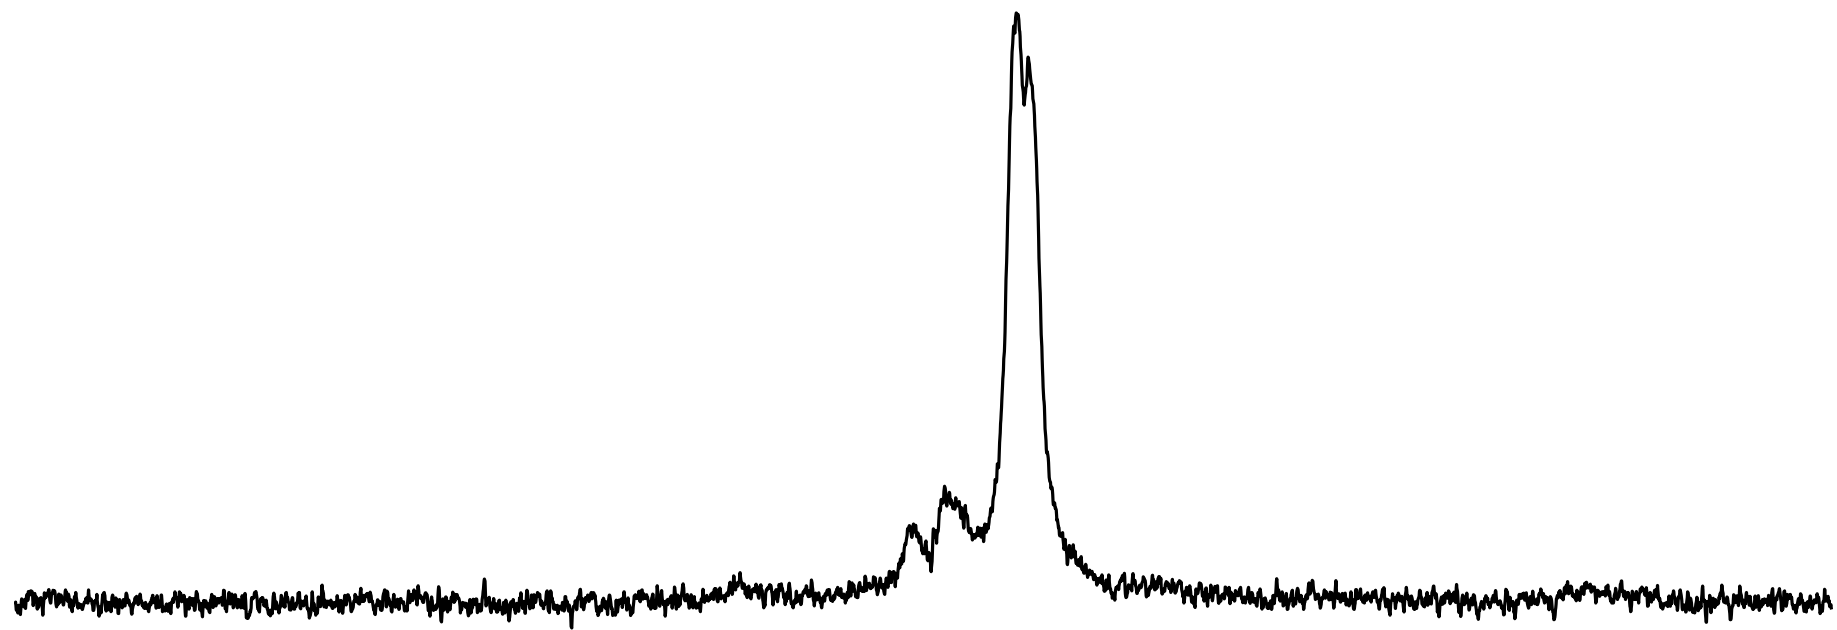

11.4 11.3 11.2 11.1 11.0 10.9 10.8 10.7 10.6 10.5 10.4 10.3 10.2 10.1 ppm

1.000

LTA in DMSO-d6
NEO 400
1D Proton Spectrum
February 25, 2025.

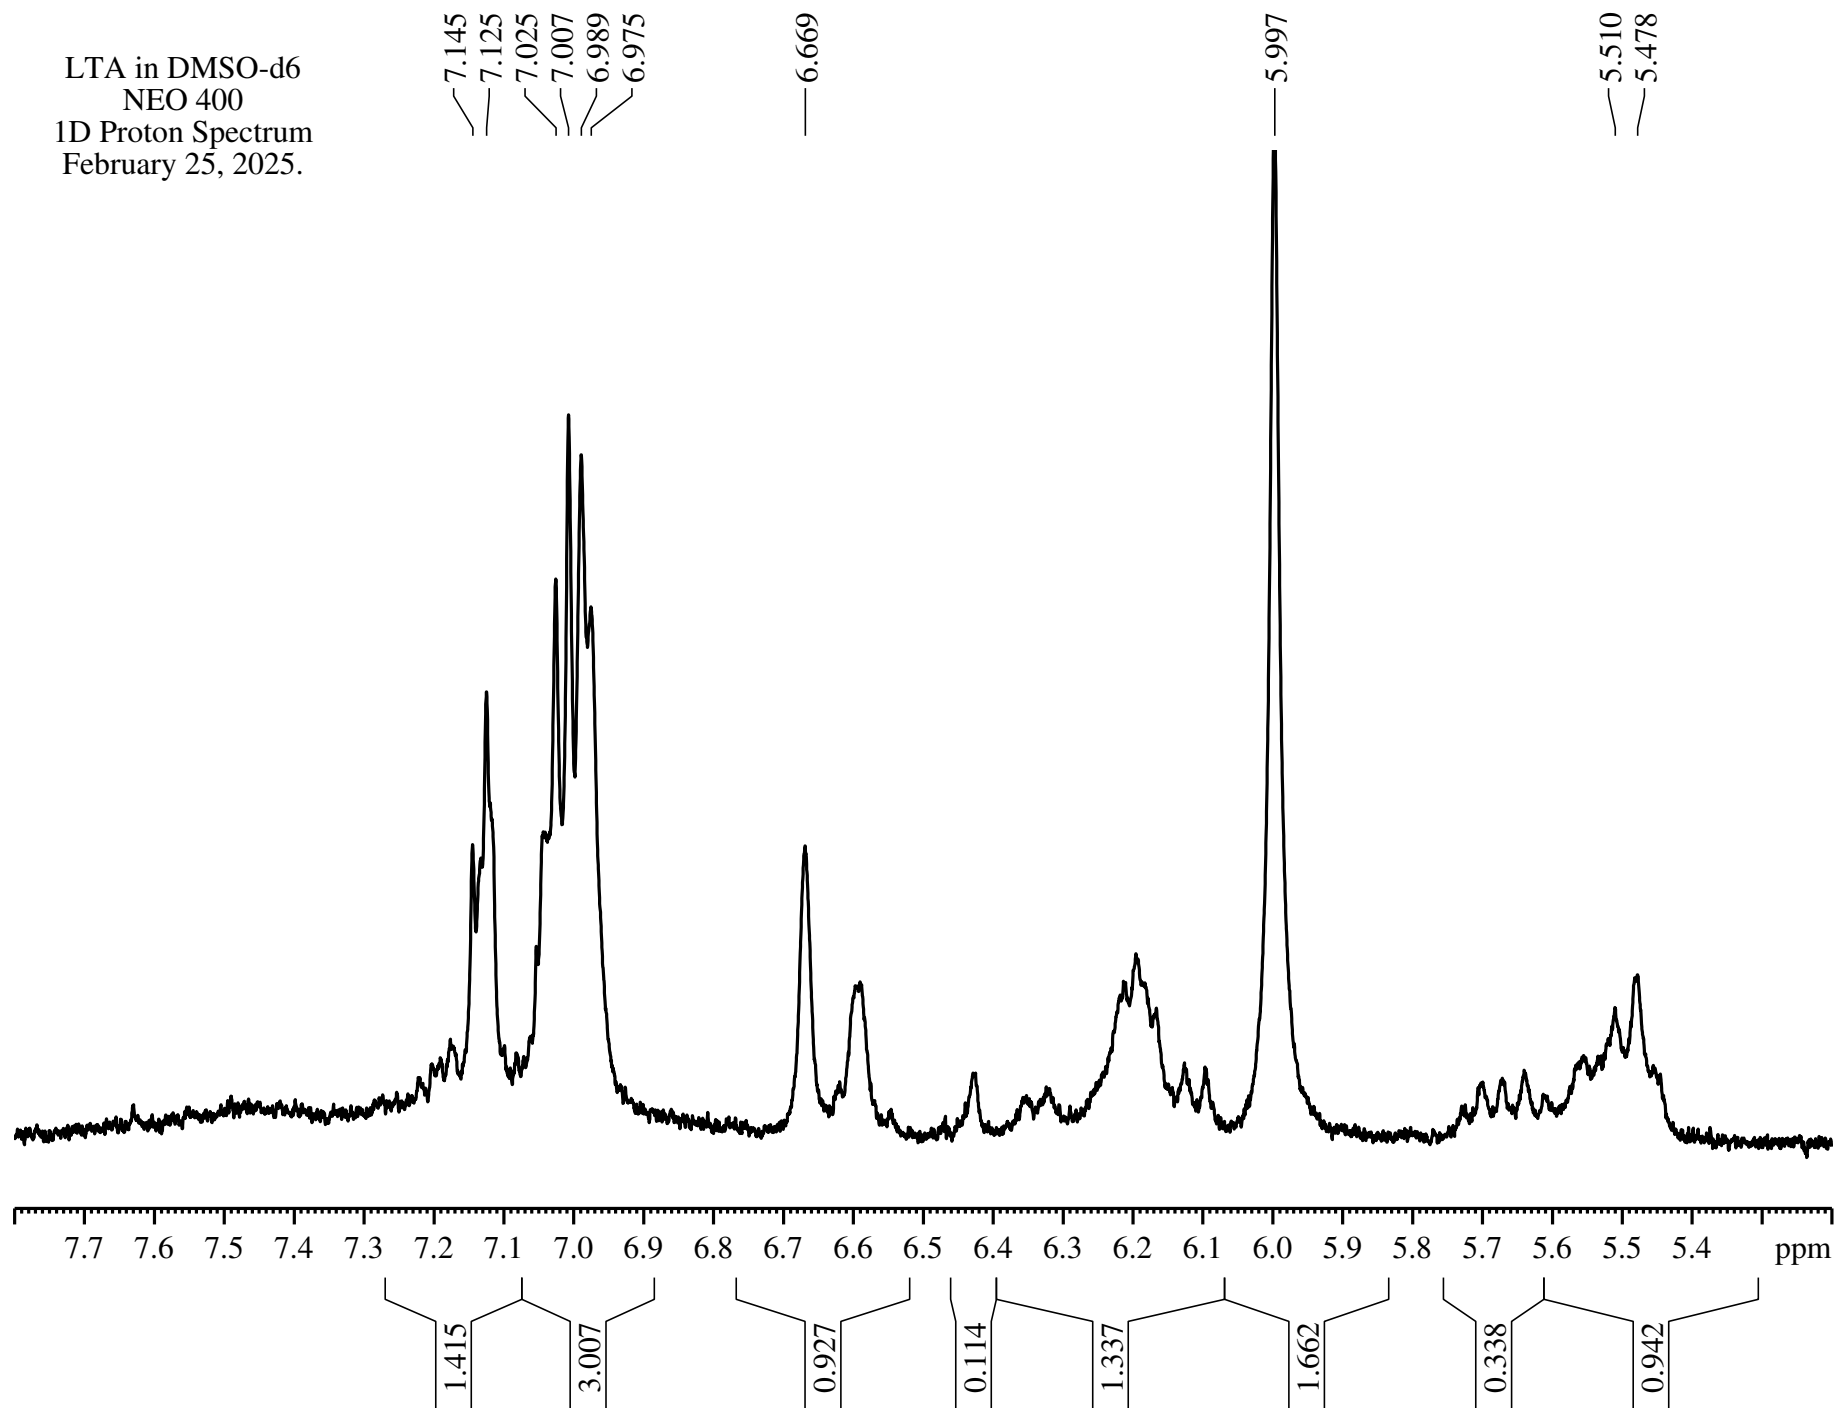

LTA in DMSO-d6
NEO 400
1D Proton Spectrum
February 25, 2025.




4.345

4.105

3.774
3.759
3.744
3.729
3.682

3.331


3.154

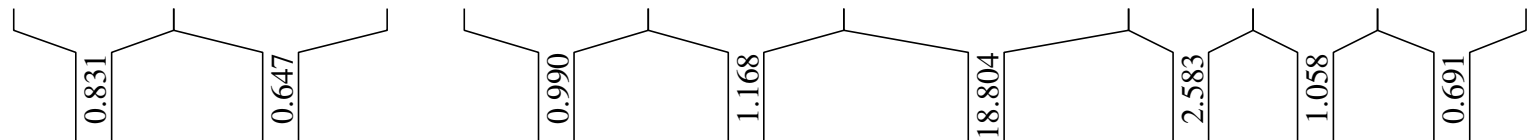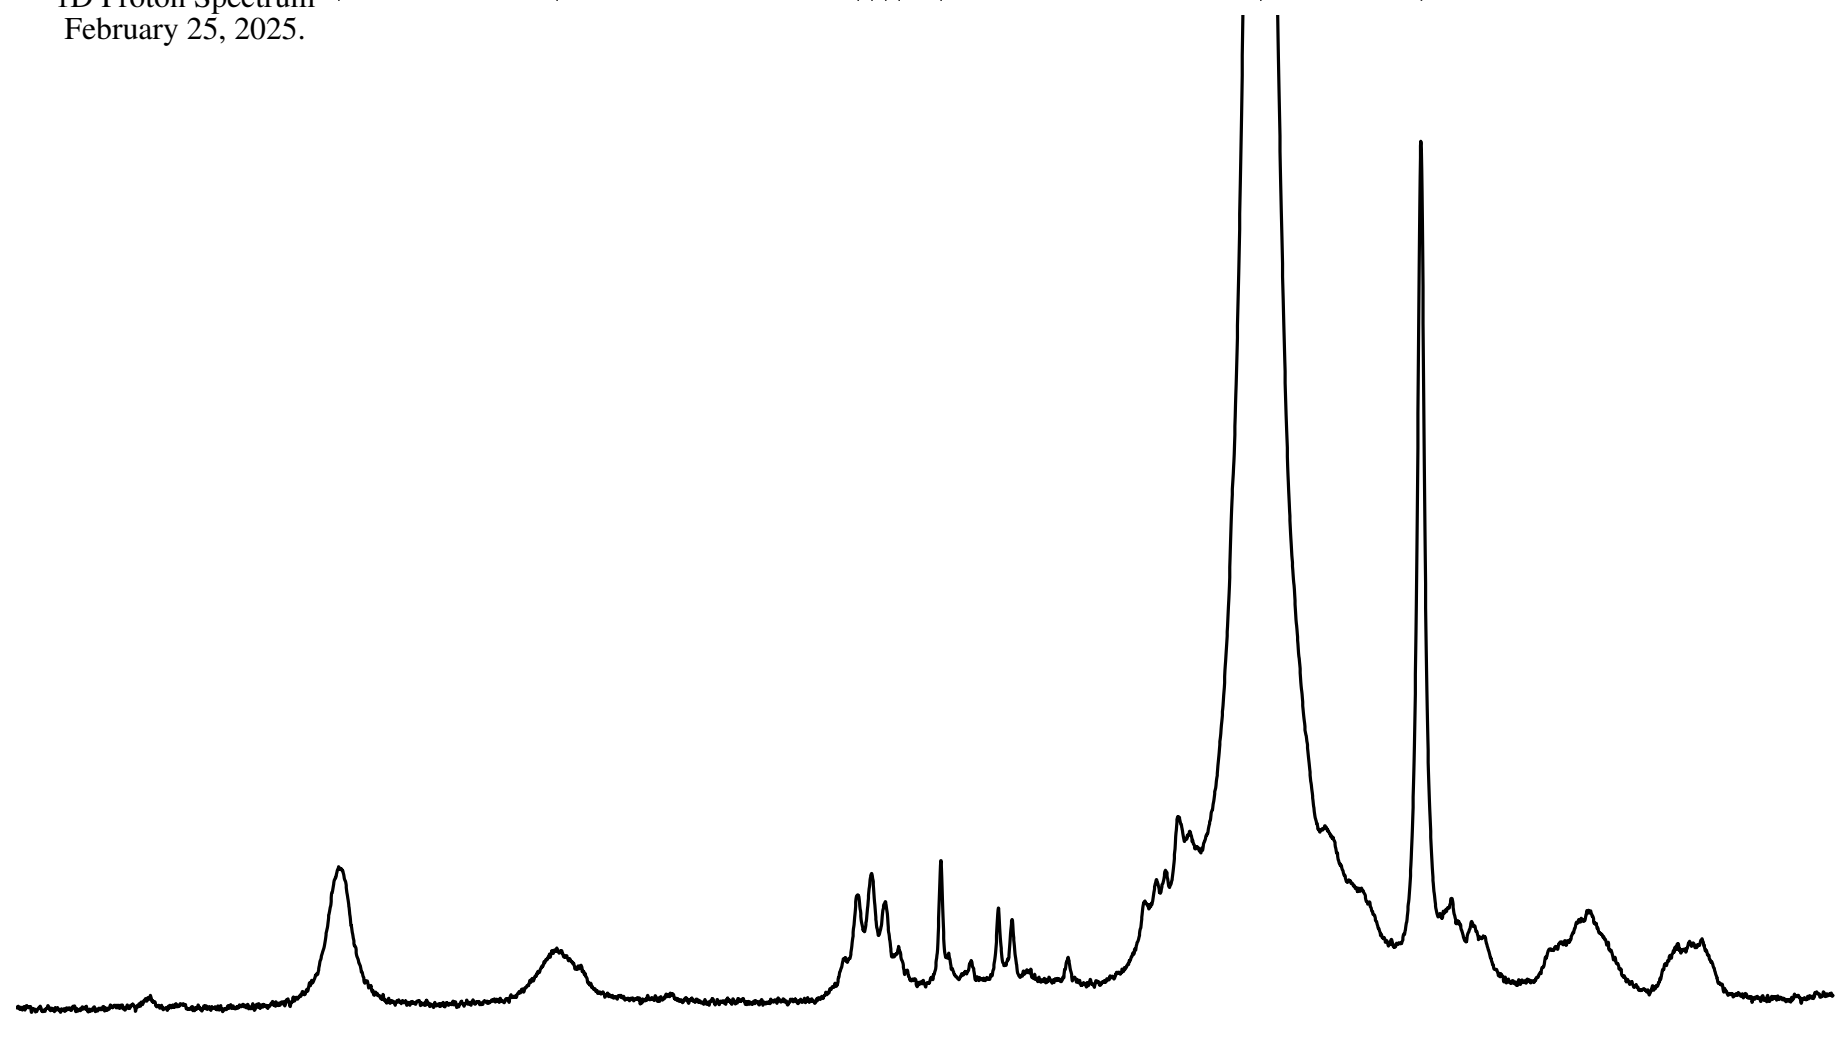

2.490
2.468
2.457
2.433
2.410

LTA in DMSO-d6
NEO 400
1D Proton Spectrum
February 25, 2025.

1.152
1.042
1.032
1.016
0.872
0.853

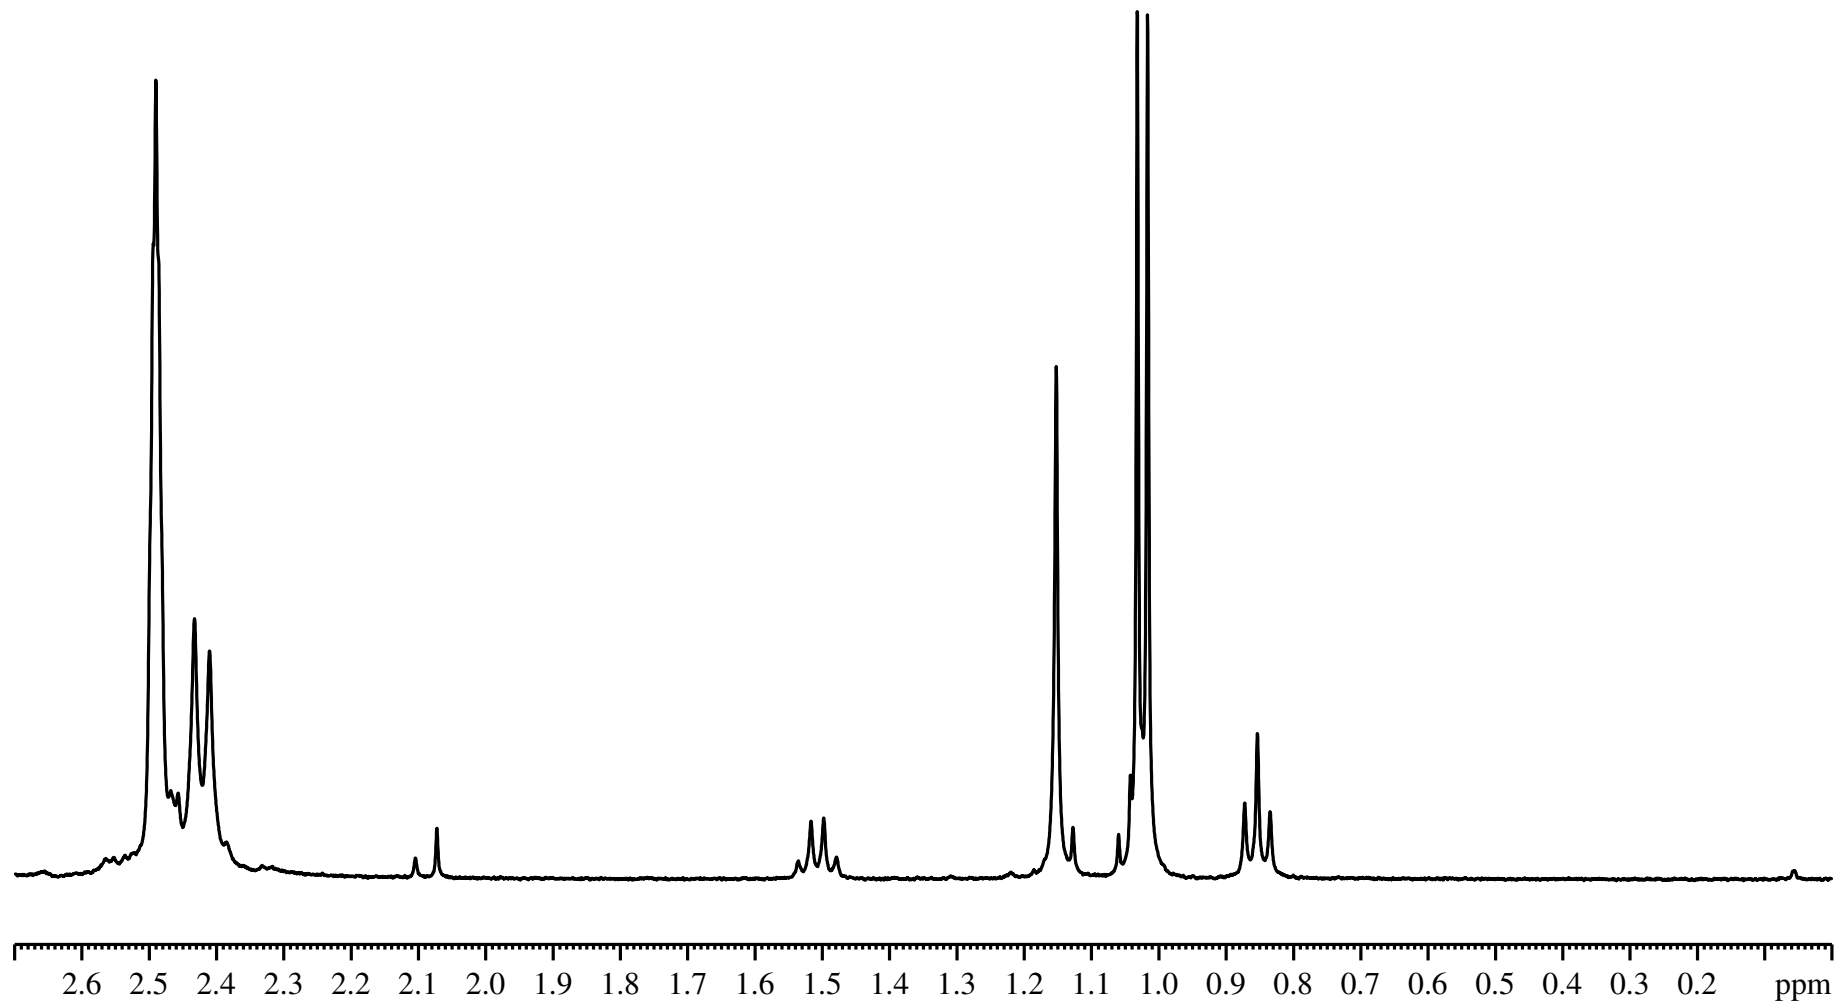

10.699

0.304

0.663

2.159

4.711

1.025