


N-iP AMT Fumarate DMSO-d6
NEO 400
1D Proton Spectrum
February 5, 2025.

Current Data Parameters
NAME Syntharise020525
EXPNO 420
PROCNO 1


F2 - Acquisition Parameters
Date_ 20250205
Time 15.03 h
INSTRUM Avance Neo 400
PROBHD Z163739_0039 (PI HR-400-S)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 0
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 295.9 K
D1 0.10000000 sec
TD0 1
SFO1 400.3424721 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 14.20300007 W

F2 - Processing parameters
SI 65536
SF 400.3400069 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

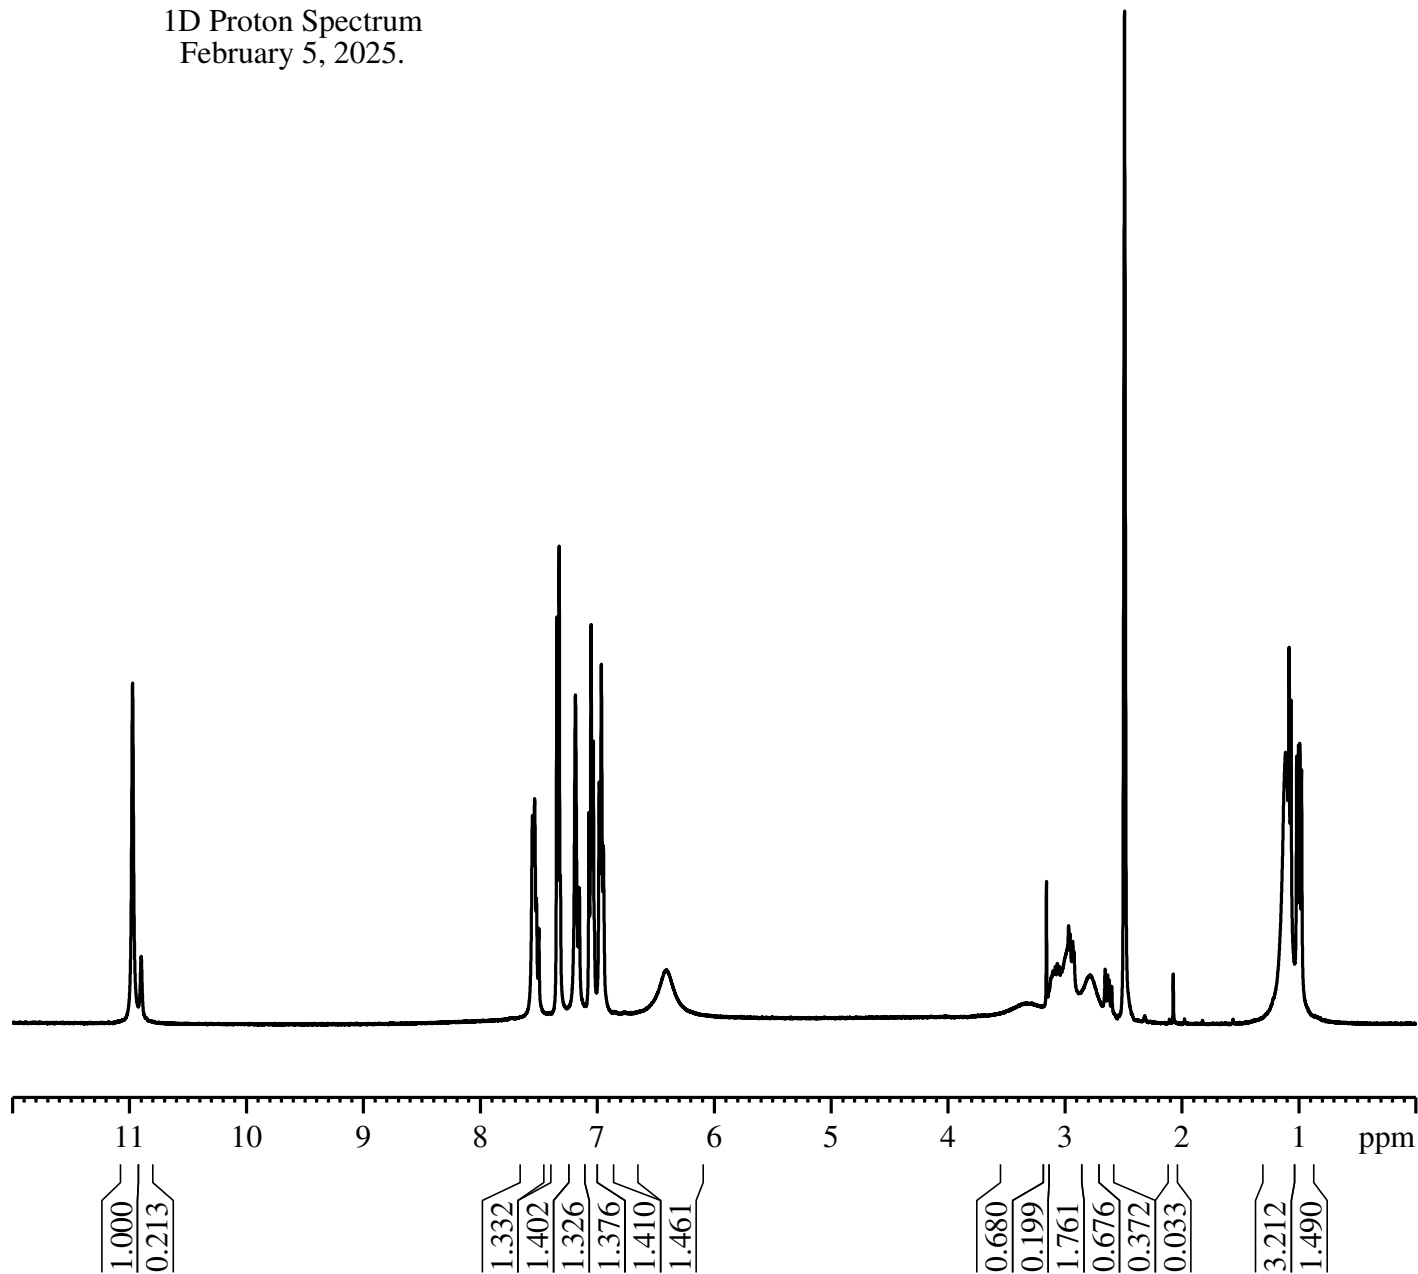

N-iP AMT Fumarate DMSO-d6
NEO 400
1D Proton Spectrum
February 5, 2025.


— 10.973
— 10.899

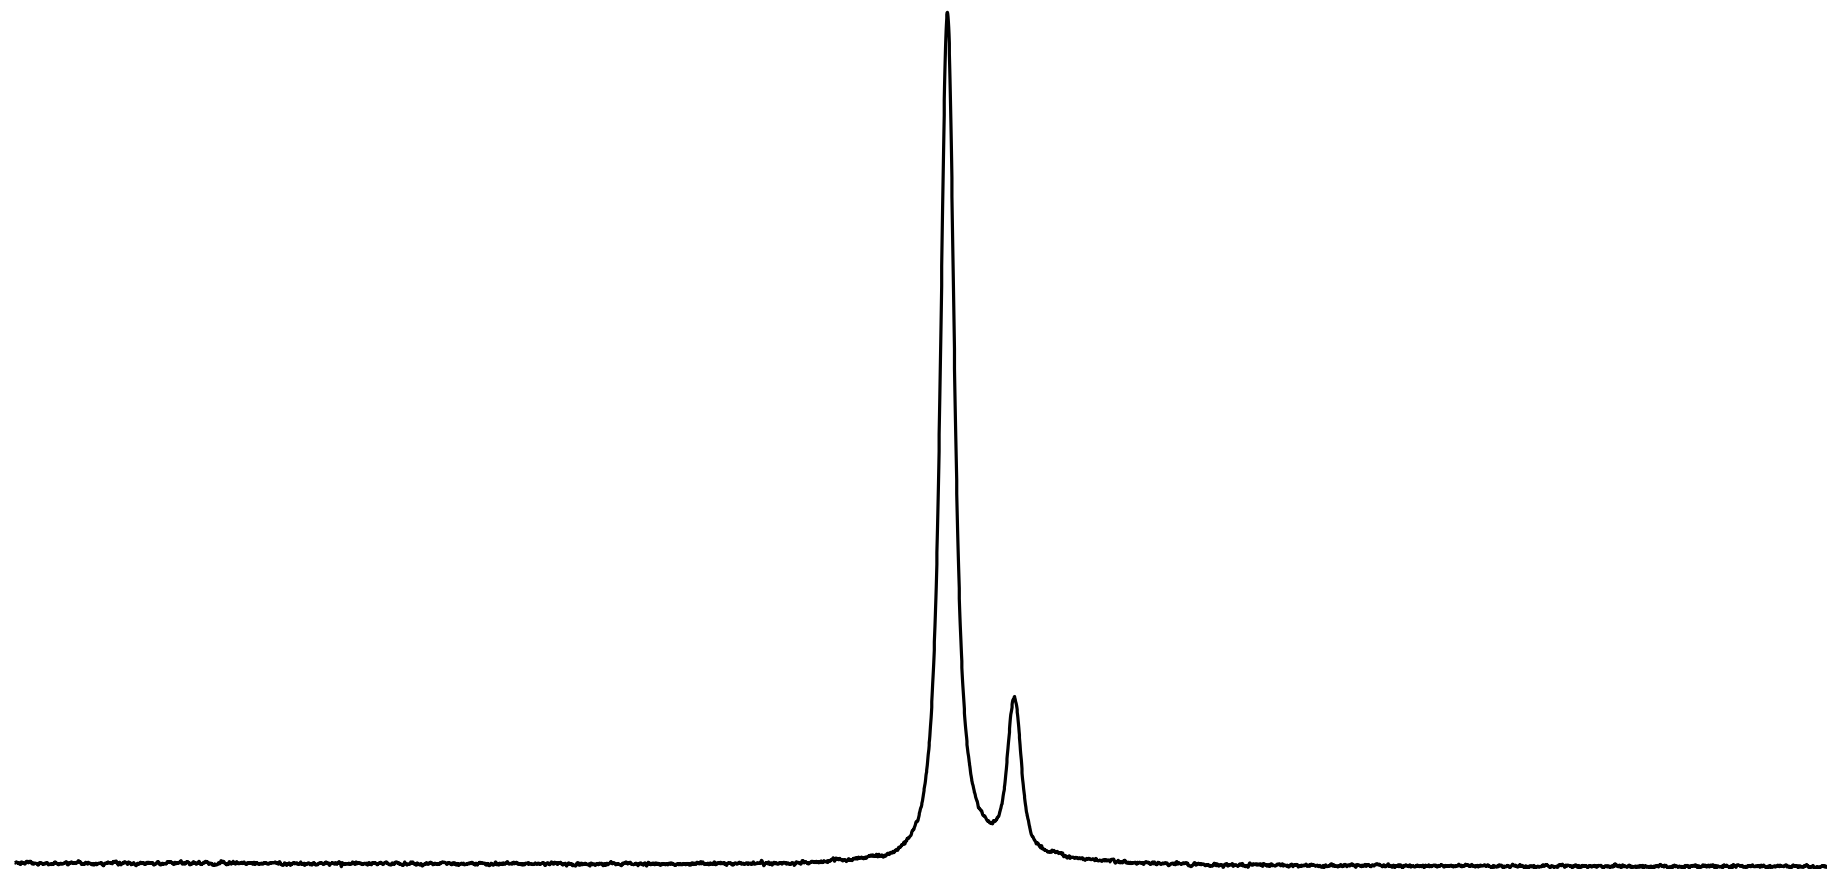

11.9 11.8 11.7 11.6 11.5 11.4 11.3 11.2 11.1 11.0 10.9 10.8 10.7 10.6 10.5 10.4 10.3 10.2 ppm

1.000 0.213

N-iP AMT Fumarate DMSO-d6
NEO 400
1D Proton Spectrum
February 5, 2025.

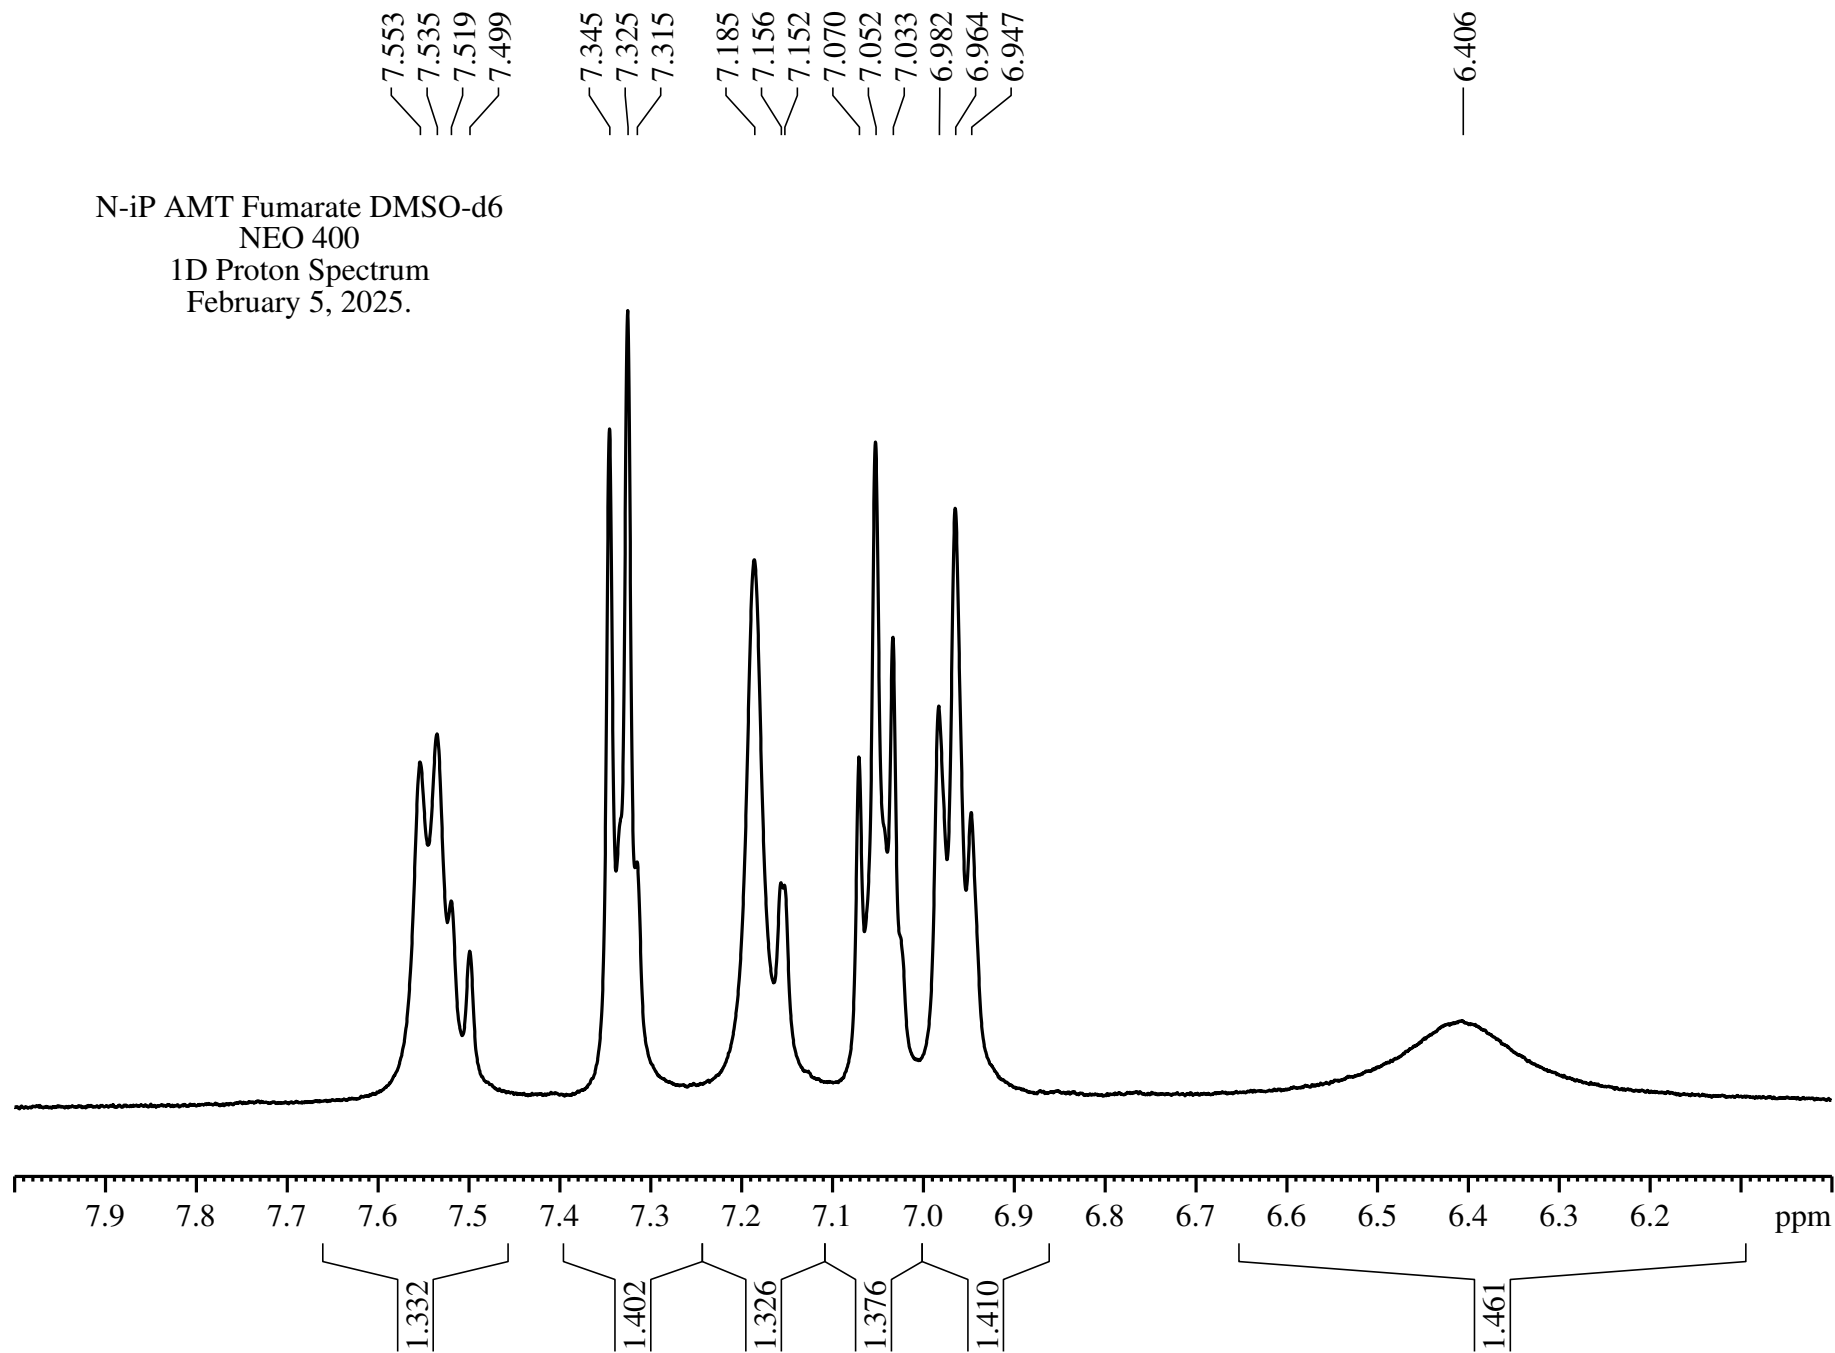

N-iP AMT Fumarate DMSO-d6
NEO 400
1D Proton Spectrum
February 5, 2025.

