


Pyrrolamphroamine HCl in DMSO-d6
March 31, 2025.
NEO 300
1D 1H Spectrum

Current Data Parameters
NAME Syntharise033125
EXPNO 320
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250331
Time 12.51 h
INSTRUM Neo
PROBHD Z862701_0073 (PA BBO 300)
PULPROG zg30
TD 32768
SOLVENT DMSO
NS 16
DS 0
SWH 5882.353 Hz
FIDRES 0.359030 Hz
AQ 2.7852800 sec
RG 101
DW 85.000 usec
DE 7.81 usec
TE 295.8 K
D1 1.1000002 sec
TD0 1
SFO1 300.1318533 MHz
NUC1 1H
P0 5.50 usec
P1 16.50 usec
PLW1 7.44680023 W

F2 - Processing parameters
SI 16384
SF 300.1300052 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

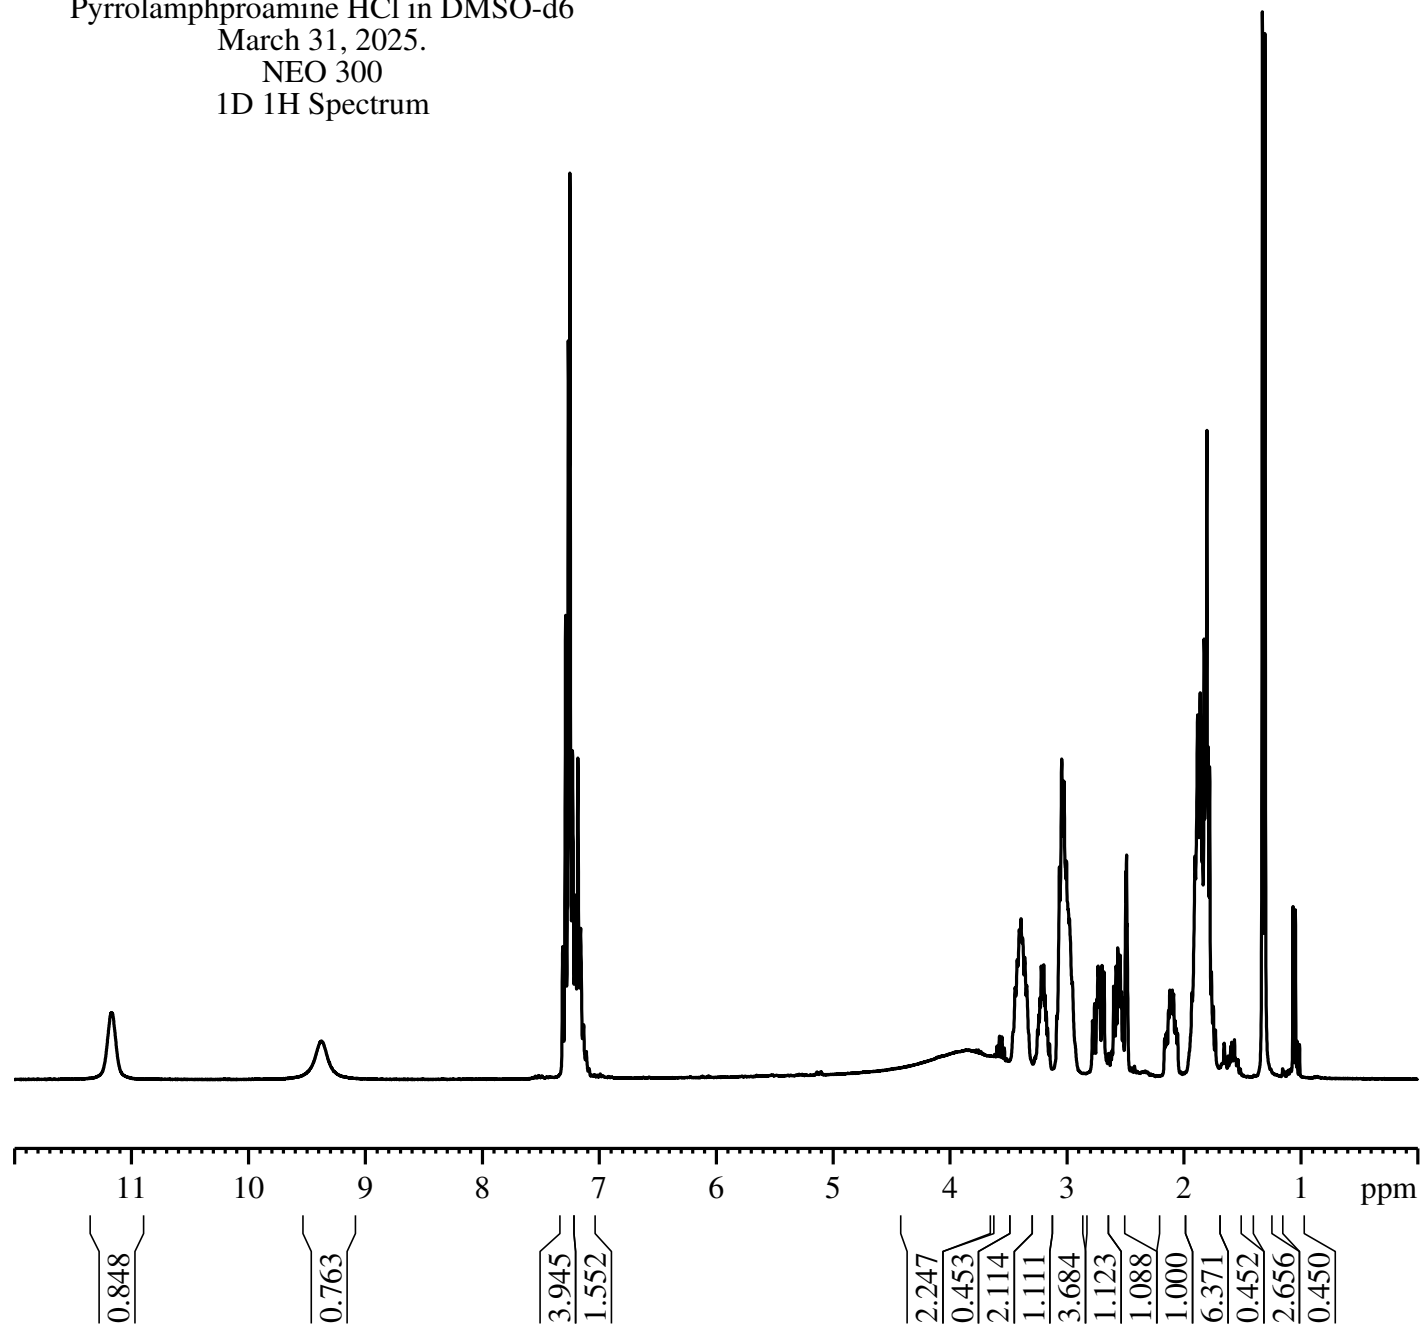


— 11.168

Pyrrolamphproamine HCl in DMSO-d6
March 31, 2025.
NEO 300
1D 1H Spectrum

— 9.374

7.286
7.263
7.249
7.227
7.181

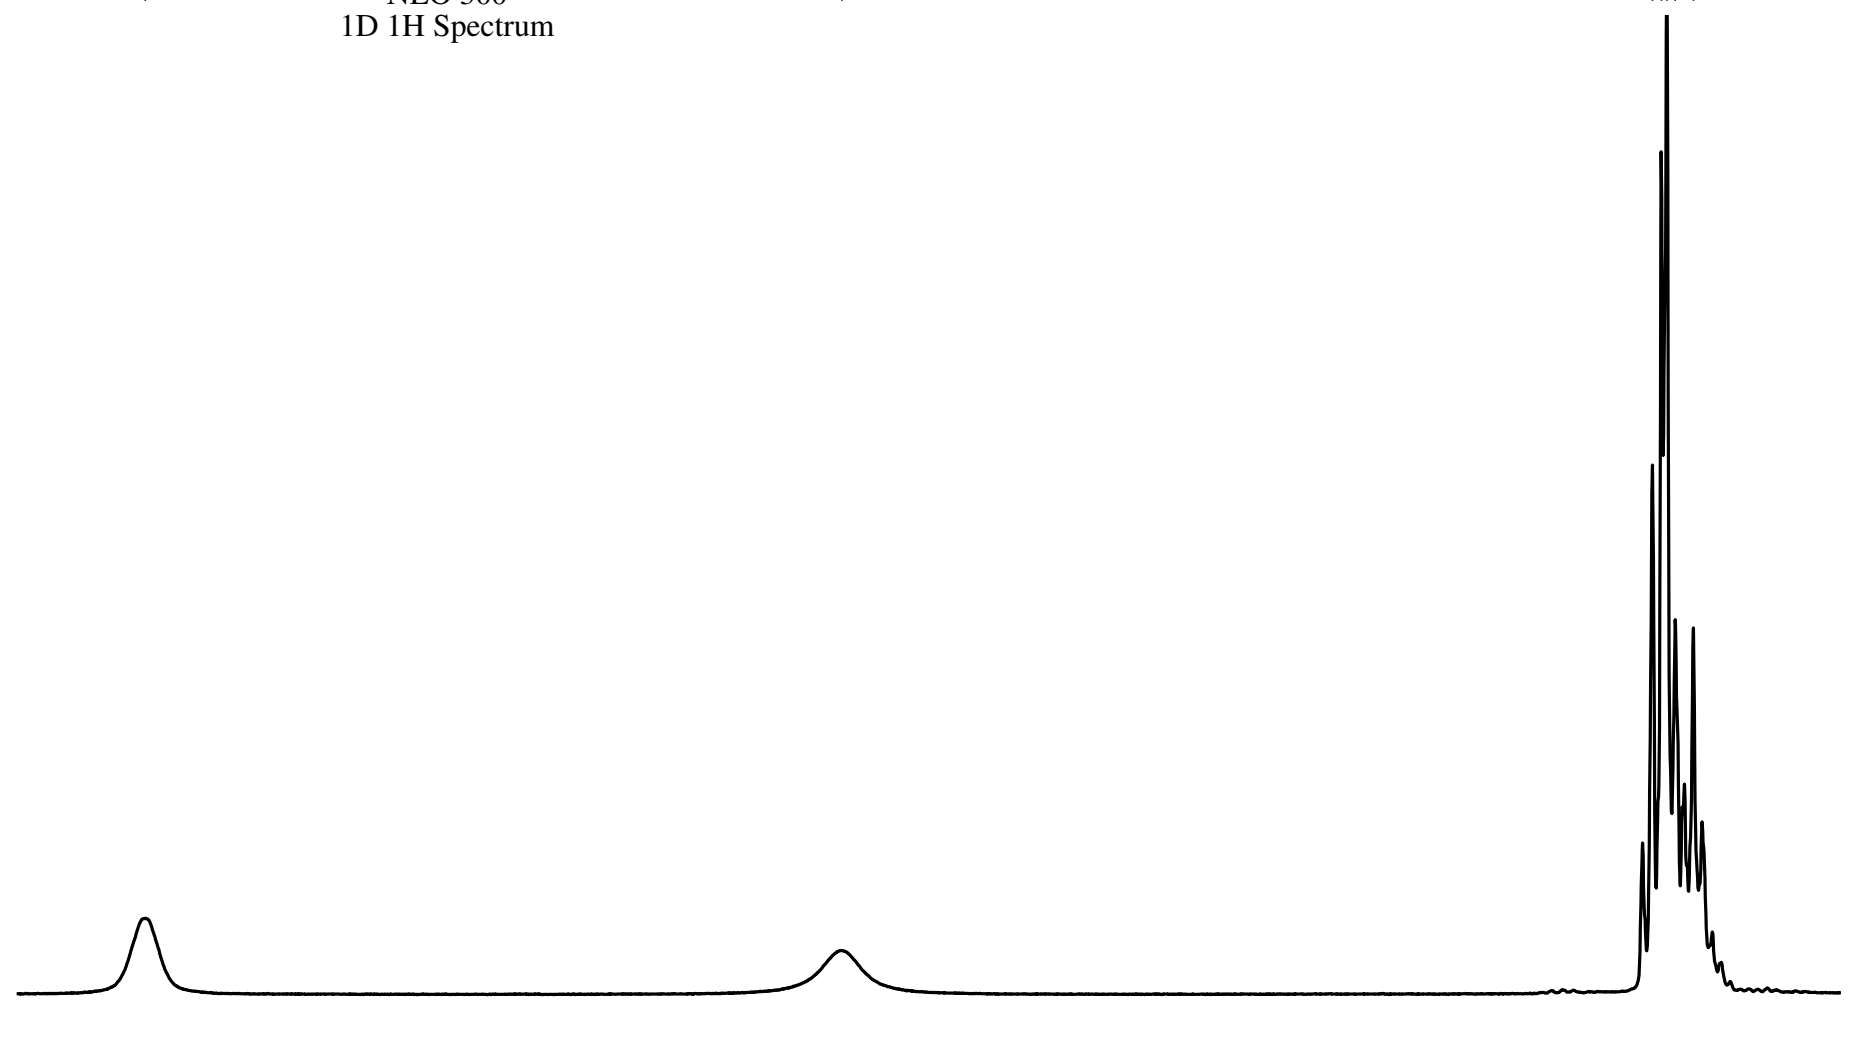

0.848

0.763


3.945

1.552

ppm

Pyrrolamphproamine HCl in DMSO-d6
March 31, 2025.
NEO 300
1D 1H Spectrum

3.424
3.407
3.392
3.378
3.360
3.218
3.208
3.197
3.063
3.043
3.025
3.003
2.988
2.977
2.951

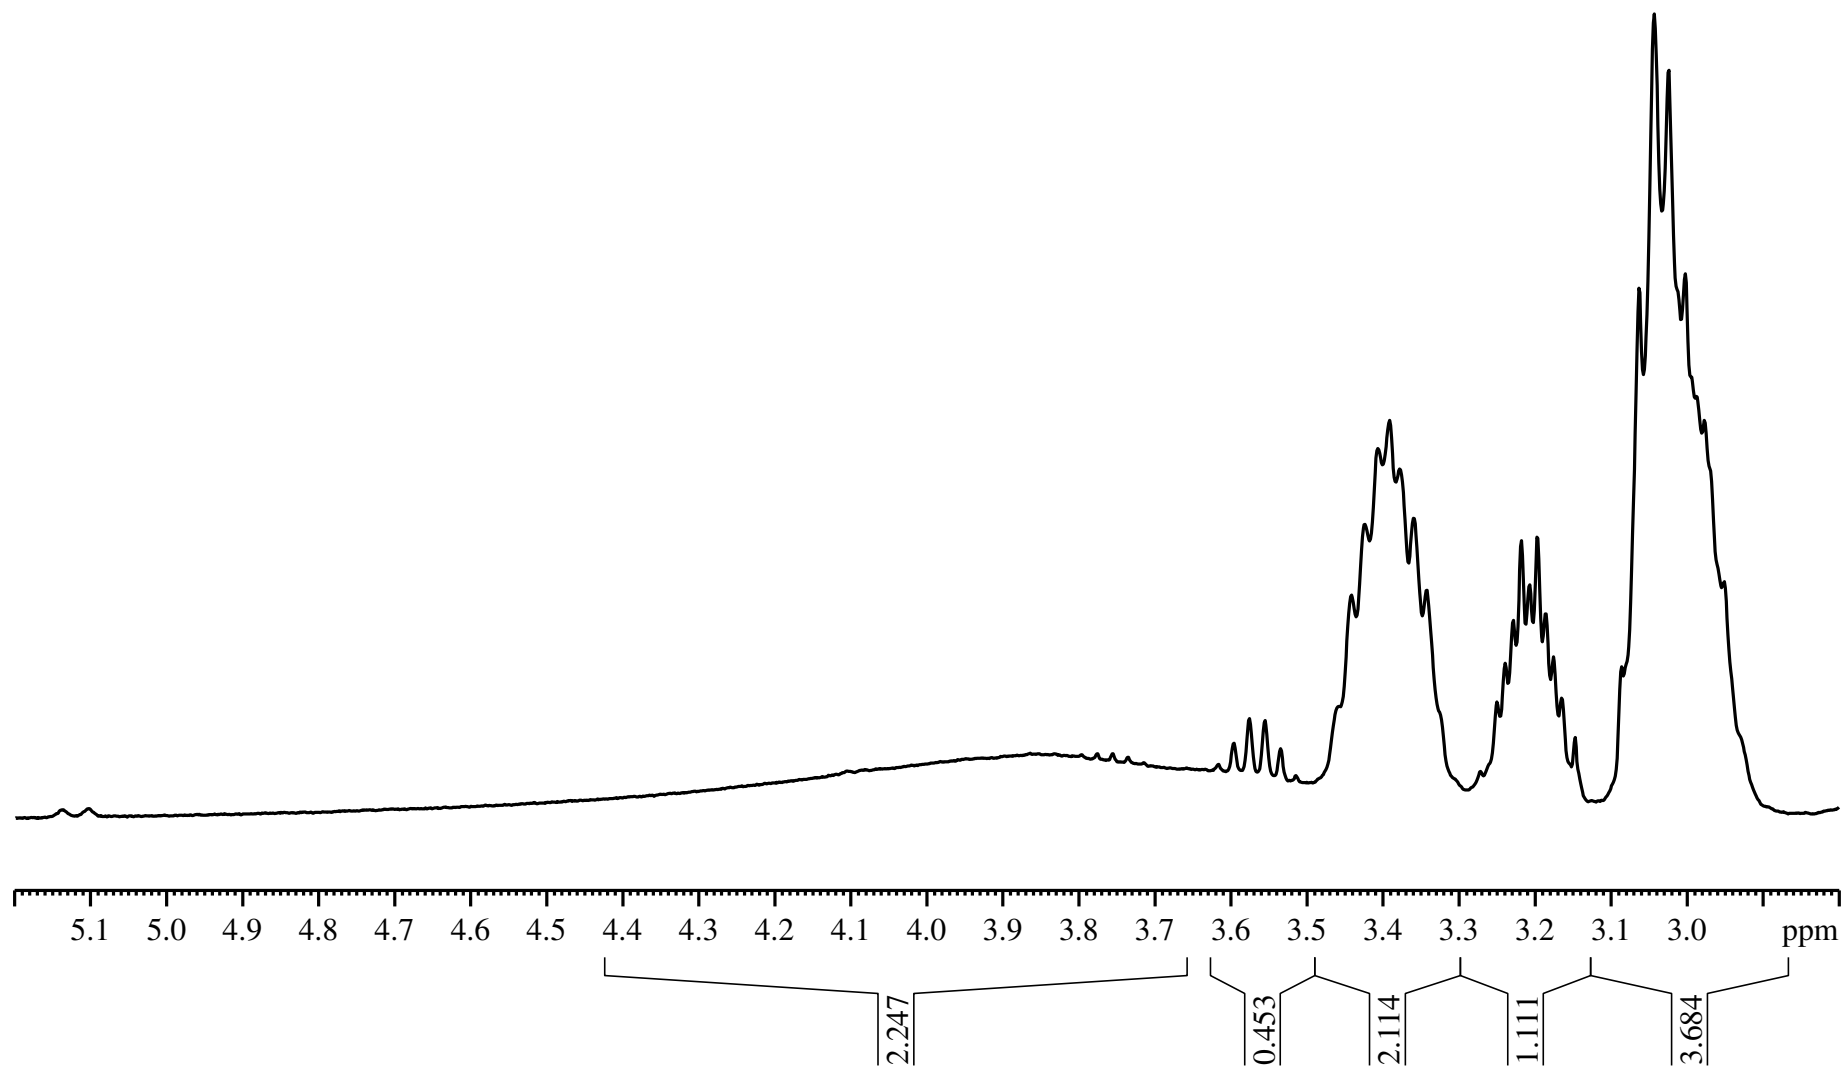


2.734
2.718
2.699
2.682
2.578
2.565
2.544
2.496
2.490
2.484

1.904
1.881
1.859
1.840
1.825
1.813
1.802
1.791
1.779
1.763

1.327
1.306

1.066
1.045

Pyrolamphproamine HCl in DMSO-d6
March 31, 2025.
NEO 300
1D 1H Spectrum

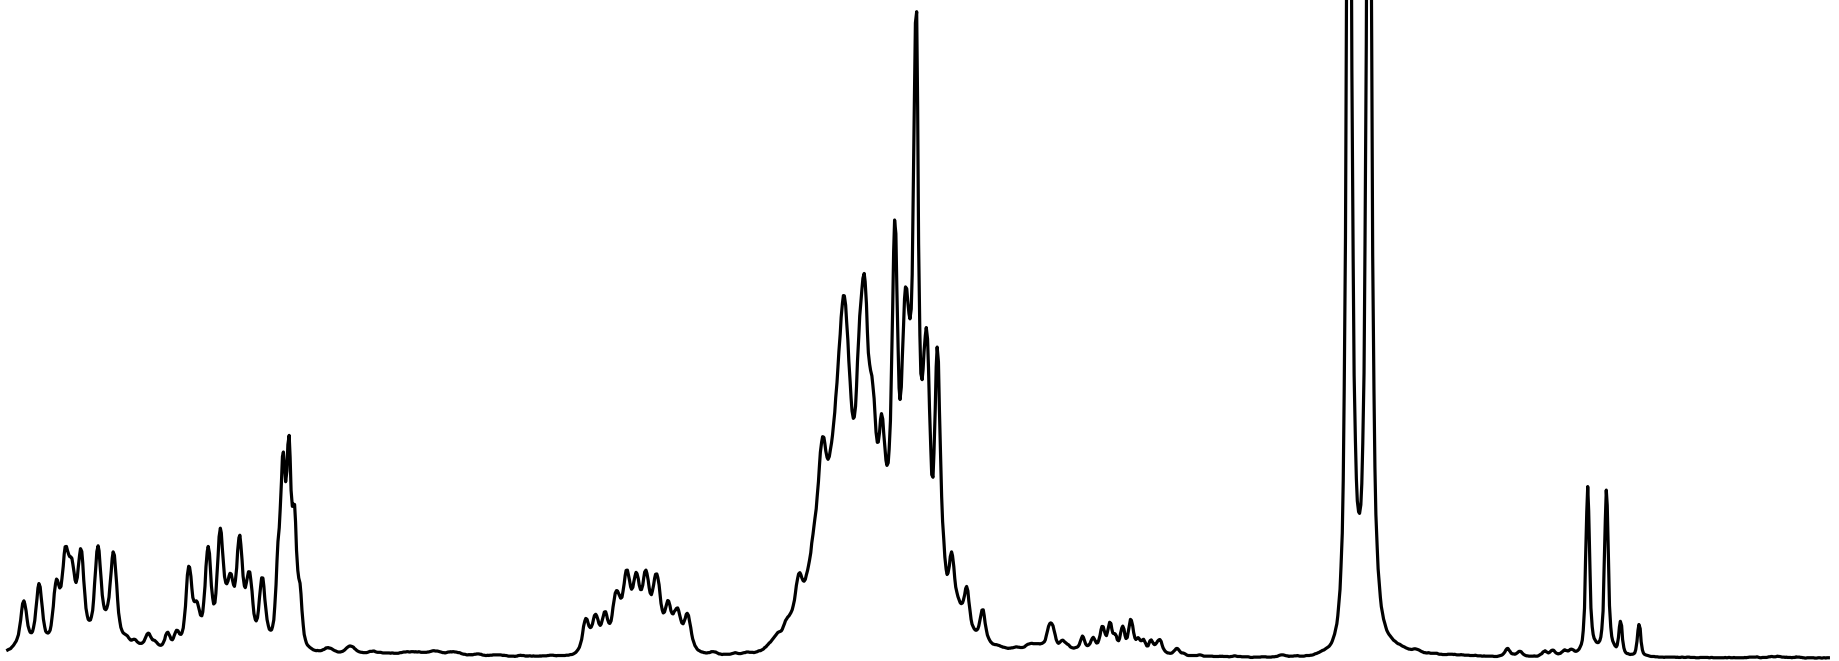

2.7 2.6 2.5 2.4 2.3 2.2 2.1 2.0 1.9 1.8 1.7 1.6 1.5 1.4 1.3 1.2 1.1 1.0 0.9 ppm

1.123
1.088

1.000
6.371
0.452

2.656

0.450