


Sample 4 2-fluoro- in DMSO-d6
July 15, 2025.
NEO 300
1D Proton Spectrum

Current Data Parameters
NAME Syntharise071525
EXPNO 330
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250715
Time 13.04 h
INSTRUM Neo
PROBHD Z862701_0073 (PA BBO 300)
PULPROG zg30
TD 32768
SOLVENT DMSO
NS 16
DS 0
SWH 5882.353 Hz
FIDRES 0.359030 Hz
AQ 2.7852800 sec
RG 101
DW 85.000 usec
DE 7.81 usec
TE 298.4 K
D1 1.1000002 sec
TD0 1
SFO1 300.1318533 MHz
NUC1 1H
P0 5.50 usec
P1 16.50 usec
PLW1 7.44680023 W


F2 - Processing parameters
SI 16384
SF 300.1300052 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

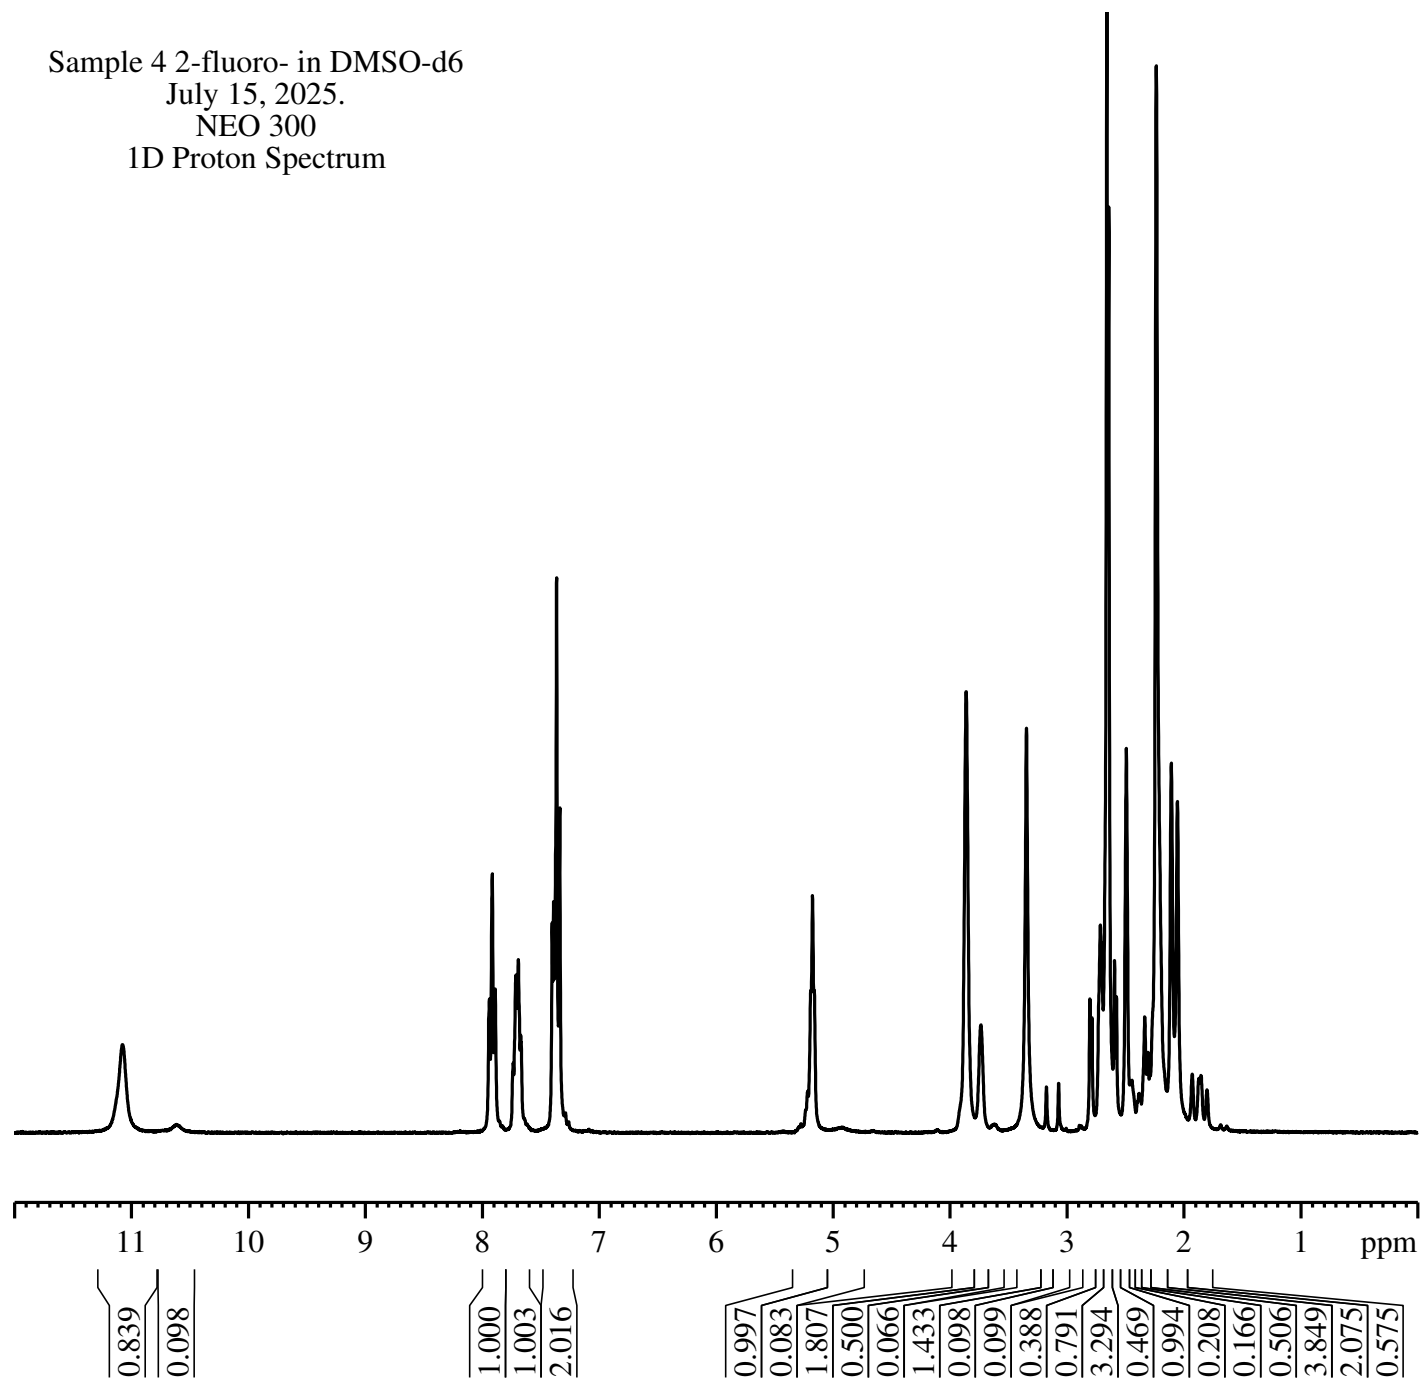

Sample 4 2-fluoro- in DMSO-d6
July 15, 2025.
NEO 300
1D Proton Spectrum

— 11.074

— 10.616

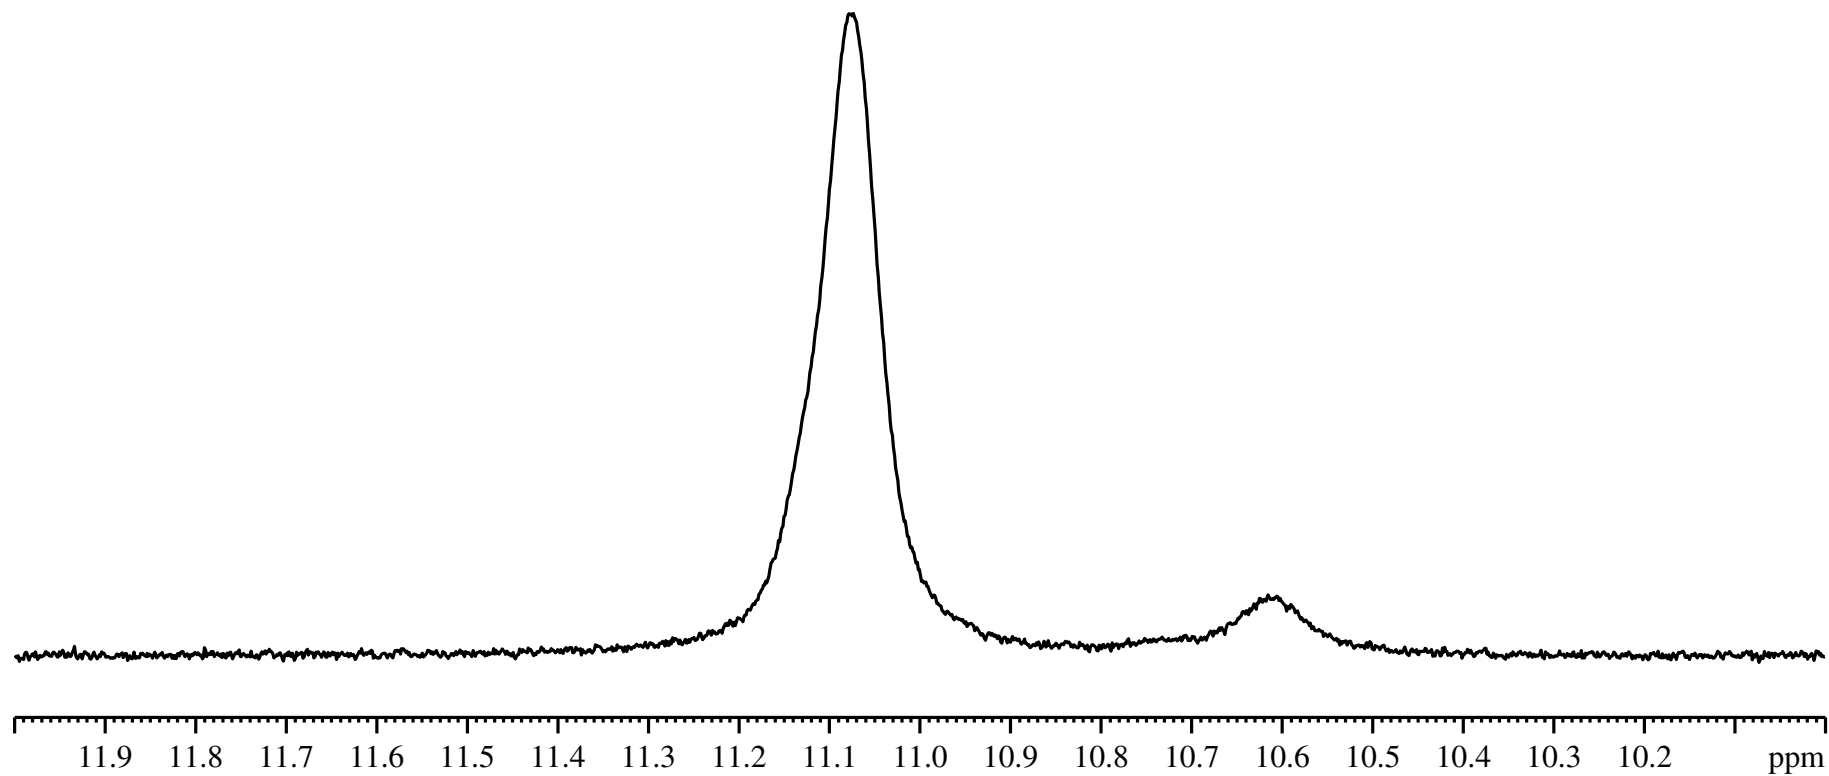


0.839 0.098

— 7.939
— 7.913
— 7.888

— 7.735
— 7.711
— 7.691
— 7.671

— 7.401
— 7.389
— 7.363
— 7.337

Sample 4 2-fluoro- in DMSO-d6
July 15, 2025.
NEO 300
1D Proton Spectrum

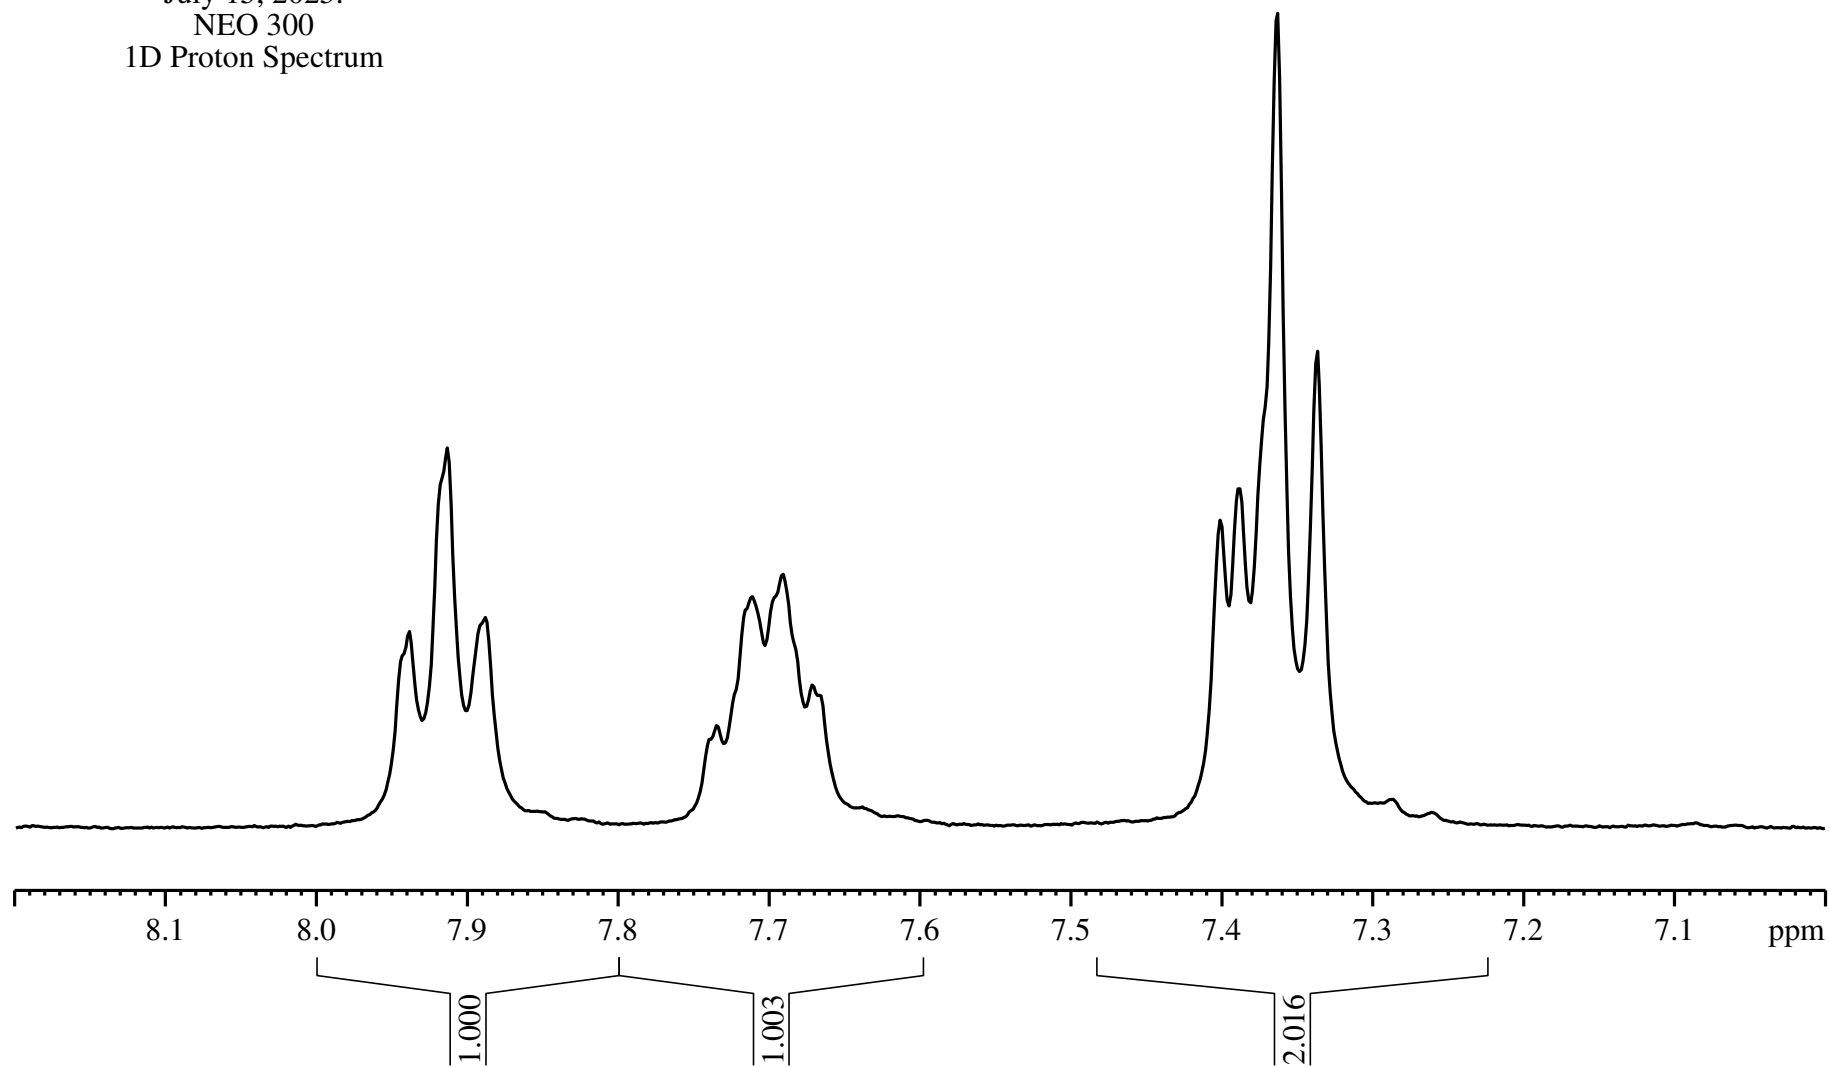

5.217
5.189
5.175
5.161

3.861


3.735

3.345

3.174

3.070

Sample 4 2-fluoro- in DMSO-d6
July 15, 2025.
NEO 300
1D Proton Spectrum

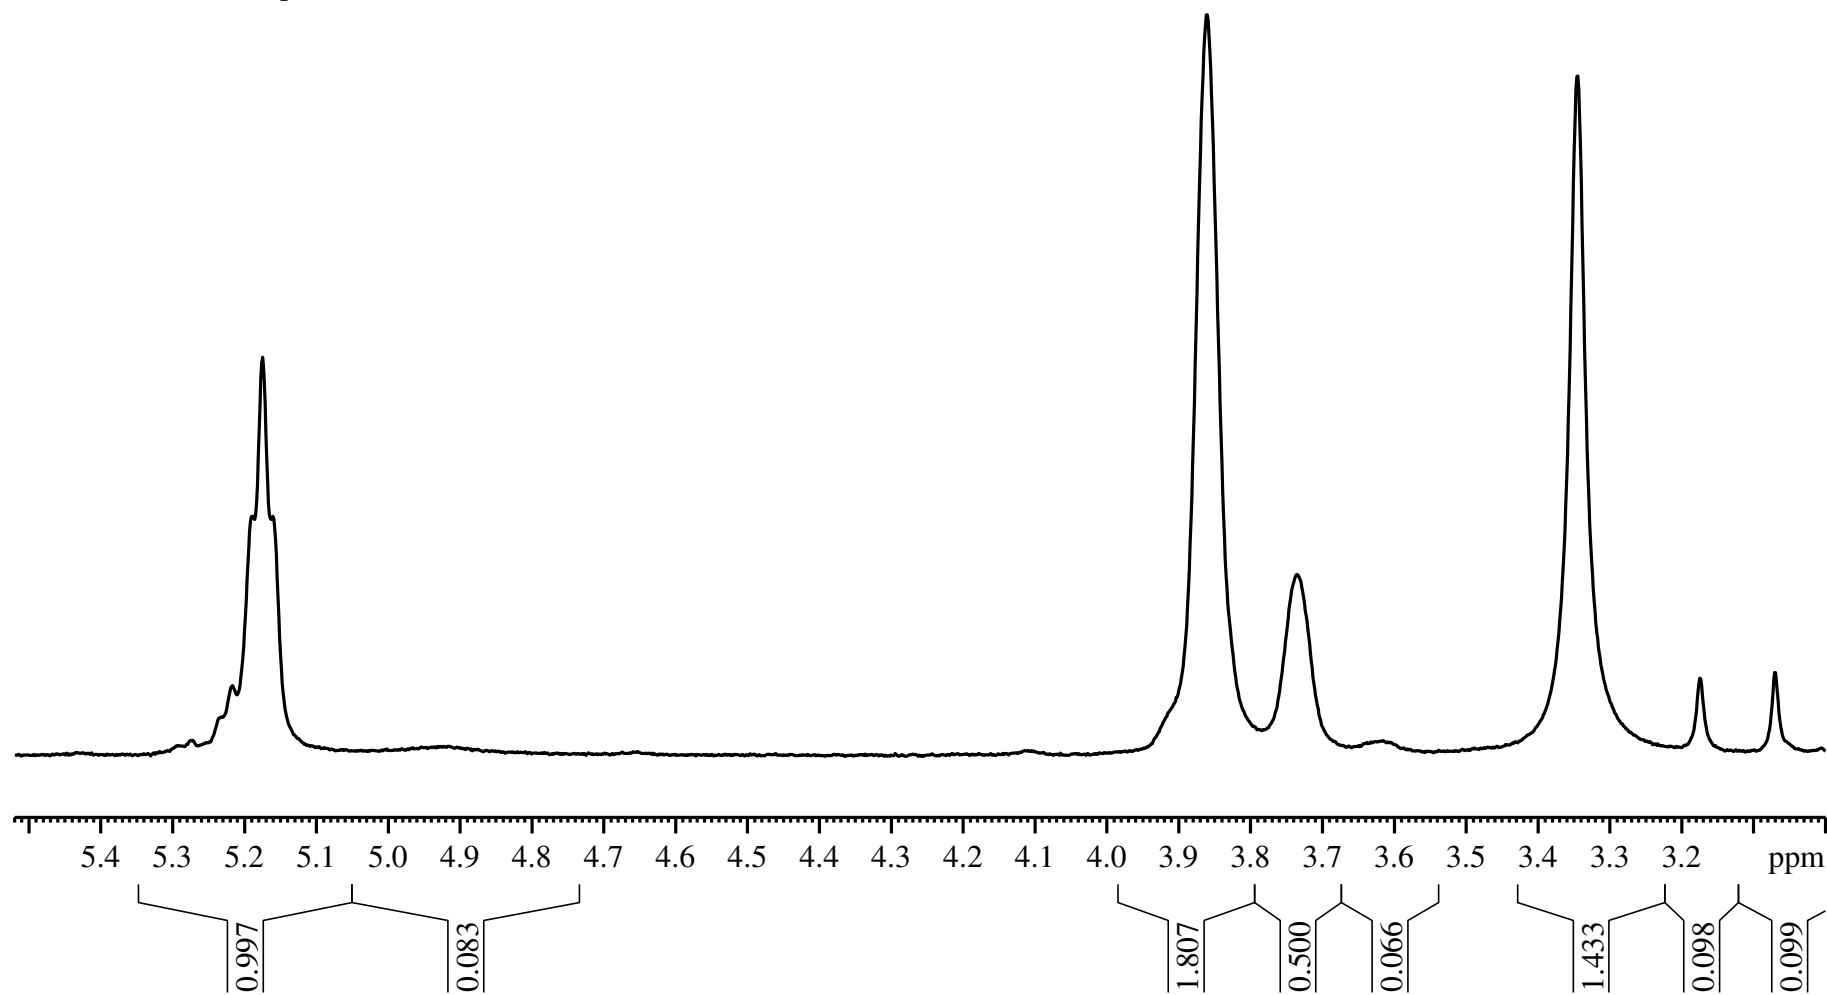

Sample 4 2-fluoro- in DMSO-d6
July 15, 2025.
NEO 300
1D Proton Spectrum

